

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
 Data File : VU063241.D
 Acq On : 11 Feb 2025 17:26
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Quant Time: Feb 12 03:21:23 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Feb 11 08:42:19 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Fluorobenzene	6.107	96	49048	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.631	95	14006	0.866	ug/l	0.00
Spiked Amount 1.000			Recovery	=	87.000%	
68) 1,2-Dichlorobenzene-d4	12.187	152	13783	0.819	ug/l	0.00
Spiked Amount 1.000			Recovery	=	82.000%	
Target Compounds						
90) 1,2,3-Trichlorobenzene	14.328	180	9137	0.703	ug/l	Qvalue 95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
Data File : VU063241.D
Acq On : 11 Feb 2025 17:26
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Time: Feb 12 03:21:23 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Feb 11 08:42:19 2025
Response via : Initial Calibration




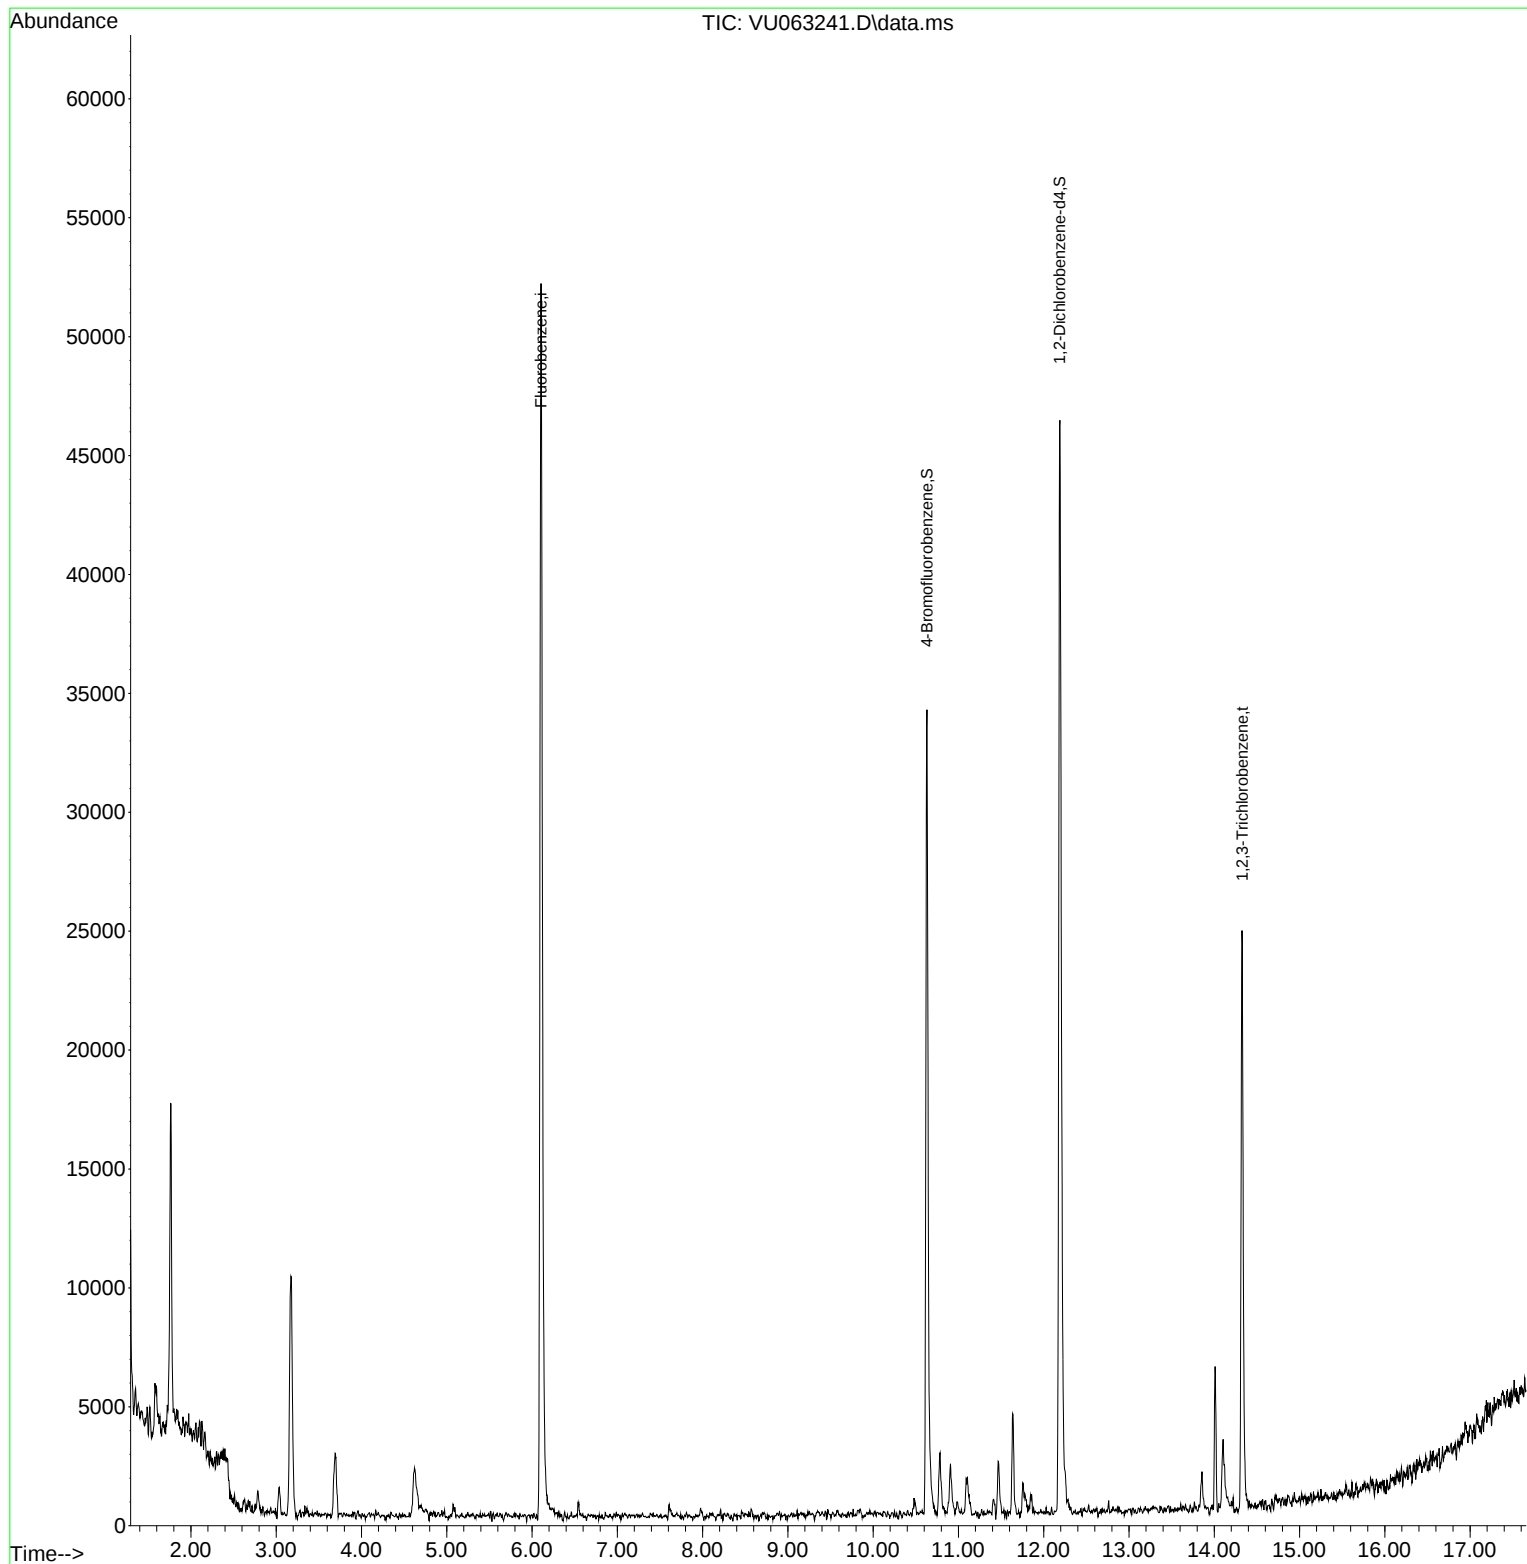


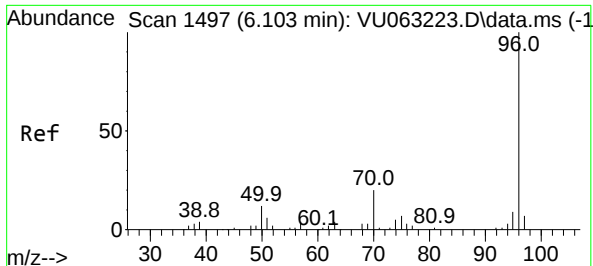

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.107 min Scan# 1498
Delta R.T. 0.004 min
Lab File: VU063241.D
Acq: 11 Feb 2025 17:26




Instrument :
MSVOA_U
ClientSampleId :
VIBLK


Tgt Ion: 96	Resp: 49048
Ion Ratio	Lower Upper
96 100	
70 20.0	15.6 23.4
95 8.6	7.3 10.9
97 6.8	0.0 0.0

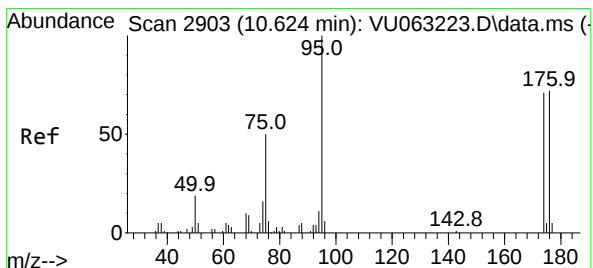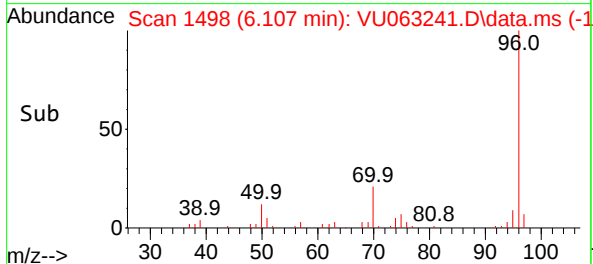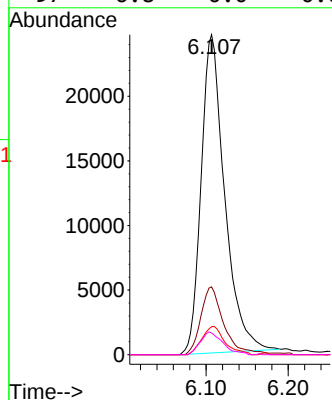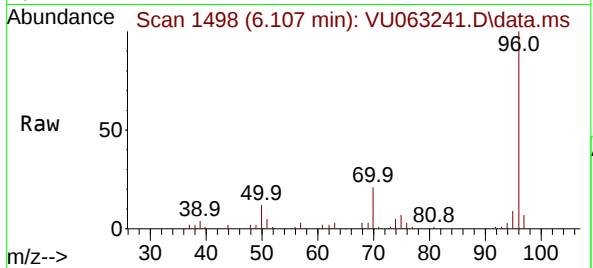

#57
4-Bromofluorobenzene
Concen: 0.866 ug/l
RT: 10.631 min Scan# 2905
Delta R.T. 0.006 min
Lab File: VU063241.D
Acq: 11 Feb 2025 17:26

Tgt Ion: 95	Resp: 14006
Ion Ratio	Lower Upper
95 100	
174 81.7	58.6 88.0
176 76.4	58.2 87.4


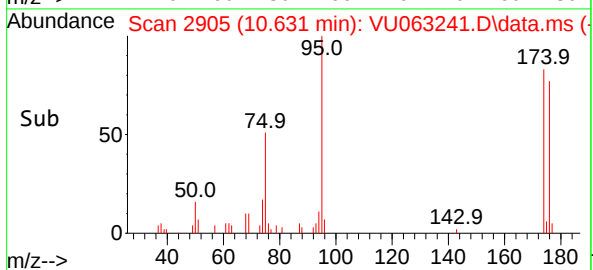
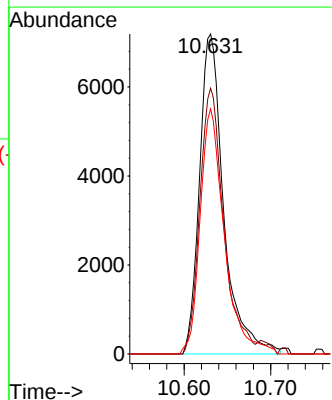
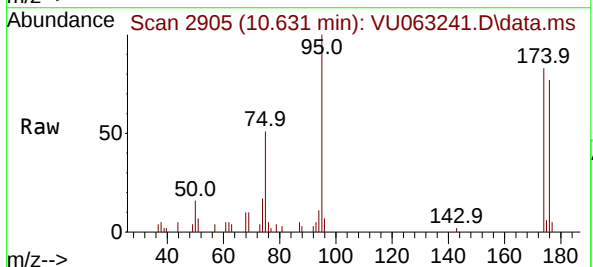


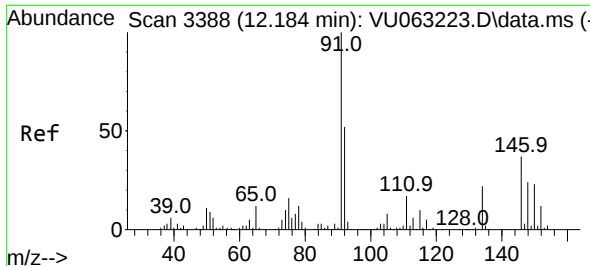

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.819 ug/l
 RT: 12.187 min Scan# 31
 Delta R.T. 0.003 min
 Lab File: VU063241.D
 Acq: 11 Feb 2025 17:26

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Tgt Ion:152 Resp: 13783
 Ion Ratio Lower Upper
 152 100
 115 67.5 0.0 275.2
 150 155.2 0.0 658.4

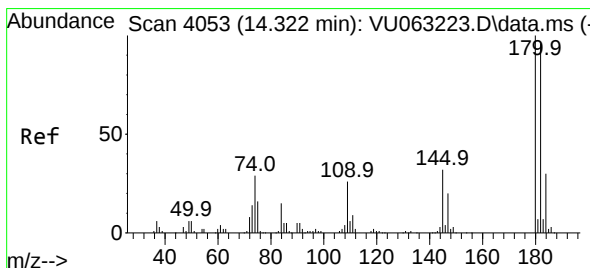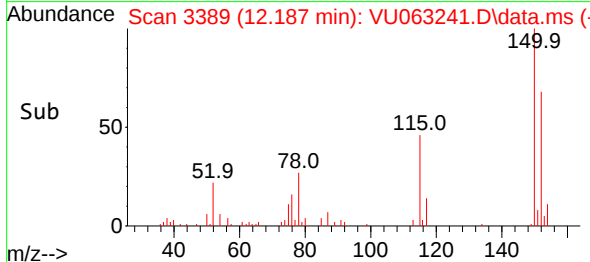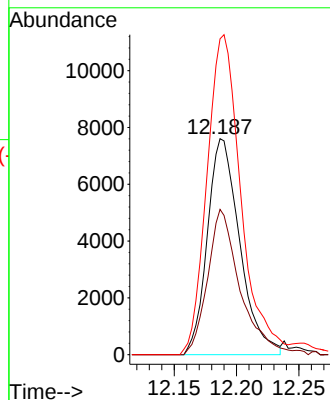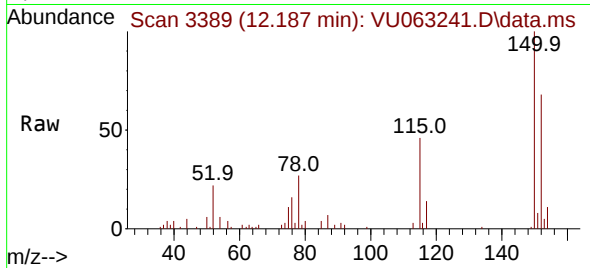

#90
 1,2,3-Trichlorobenzene
 Concen: 0.703 ug/l
 RT: 14.328 min Scan# 4055
 Delta R.T. 0.006 min
 Lab File: VU063241.D
 Acq: 11 Feb 2025 17:26

Tgt Ion:180 Resp: 9137
 Ion Ratio Lower Upper
 180 100
 182 92.3 78.2 117.2
 145 31.4 26.1 39.1

