

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
 Data File : VU063229.D
 Acq On : 11 Feb 2025 11:14
 Operator : MD/SY
 Sample : VU0211WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0211WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063229.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.827	164	167	170	rBV3	1797	1629	1.48%	0.554%
2	2.782	457	464	470	rBV2	1214	1800	1.64%	0.612%
3	3.168	577	584	593	rBV3	1117	2213	2.01%	0.752%
4	3.692	736	747	757	rBV6	2722	6366	5.80%	2.164%
5	6.107	1487	1498	1520	rBV	53201	109848	100.00%	37.333%
6	9.698	2607	2615	2620	rBV3	987	1398	1.27%	0.475%
7	10.631	2894	2905	2926	rBV	33657	65106	59.27%	22.127%
8	11.756	3249	3255	3261	rBV3	1125	1575	1.43%	0.535%
9	11.843	3275	3282	3291	rVB3	1523	2413	2.20%	0.820%
10	12.187	3378	3389	3406	rBV	44708	86212	78.48%	29.300%
11	13.463	3778	3786	3799	rVB3	759	1526	1.39%	0.519%
12	13.849	3899	3906	3917	rBV5	3186	5166	4.70%	1.756%
13	14.109	3977	3987	3988	rBV2	1961	2369	2.16%	0.805%
14	14.331	4048	4056	4066	rBV5	3153	5373	4.89%	1.826%
15	16.055	4586	4592	4599	rBV5	780	1242	1.13%	0.422%




Sum of corrected areas: 294236

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
Data File : VU063229.D
Acq On : 11 Feb 2025 11:14
Operator : MD/SY
Sample : VU0211WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0211WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

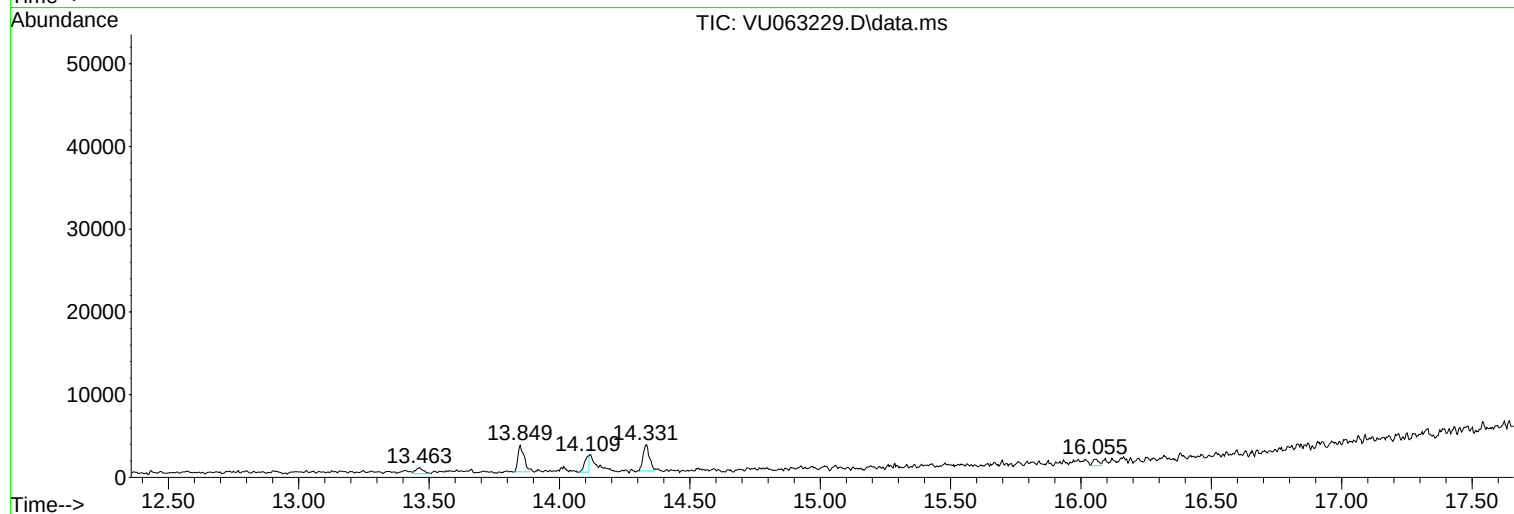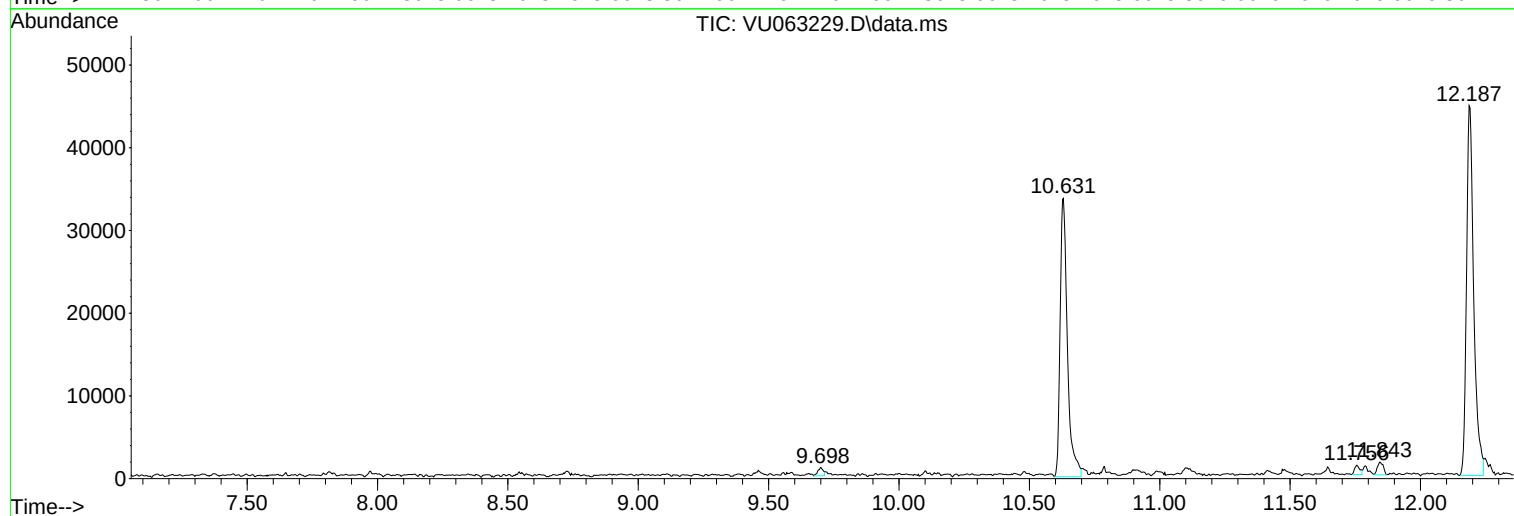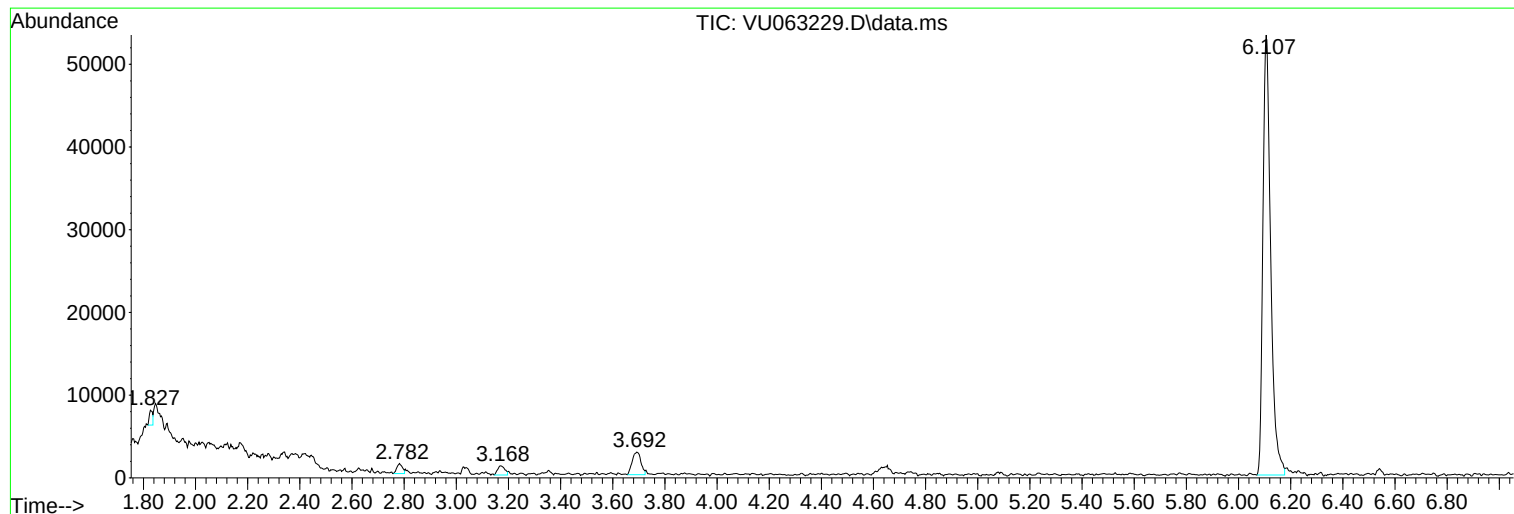

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
Data File : VU063229.D
Acq On : 11 Feb 2025 11:14
Operator : MD/SY
Sample : VU0211WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0211WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
Data File : VU063229.D
Acq On : 11 Feb 2025 11:14
Operator : MD/SY
Sample : VU0211WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0211WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------