

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
 Data File : VU063237.D
 Acq On : 11 Feb 2025 15:45
 Operator : MD/SY
 Sample : Q1172-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-RVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063237.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.570	384	398	420	rBV	428273	707505	33.11%	3.616%
2	3.030	527	541	568	rBV	526329	997051	46.66%	5.095%
3	3.171	573	585	601	rVB2	9980	24044	1.13%	0.123%
4	3.342	621	638	667	rBV	208825	424143	19.85%	2.168%
5	4.650	1021	1045	1079	rBV	542361	1258434	58.89%	6.431%
6	5.300	1230	1247	1274	rBV	261874	593252	27.76%	3.032%
7	5.512	1292	1313	1344	rBV	475025	1052761	49.26%	5.380%
8	5.766	1377	1392	1420	rBV2	198117	492436	23.04%	2.517%
9	6.103	1486	1497	1525	rBV	54600	112170	5.25%	0.573%
10	6.528	1616	1629	1662	rBV	757694	1451220	67.91%	7.416%
11	6.779	1695	1707	1742	rVB	120047	234969	11.00%	1.201%
12	7.959	2061	2074	2103	rBV	1240139	2137018	100.00%	10.921%
13	8.386	2195	2207	2227	rBV	293056	512862	24.00%	2.621%
14	8.541	2240	2255	2280	rBV	891797	1509495	70.64%	7.714%
15	9.434	2518	2533	2560	rBV	557779	944220	44.18%	4.825%
16	9.560	2560	2572	2599	rVV	506064	821232	38.43%	4.197%
17	9.682	2599	2610	2639	rVB	227633	394590	18.46%	2.017%
18	10.100	2722	2740	2785	rBV3	709898	1426035	66.73%	7.288%
19	10.627	2893	2904	2925	rBV	49543	83916	3.93%	0.429%
20	11.827	3264	3277	3301	rBV	1011834	1670640	78.18%	8.538%
21	12.200	3377	3393	3418	rBV	1007887	1751418	81.96%	8.950%
22	13.830	3887	3900	3935	rBV	566200	968614	45.33%	4.950%




Sum of corrected areas: 19568025

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
Data File : VU063237.D
Acq On : 11 Feb 2025 15:45
Operator : MD/SY
Sample : Q1172-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

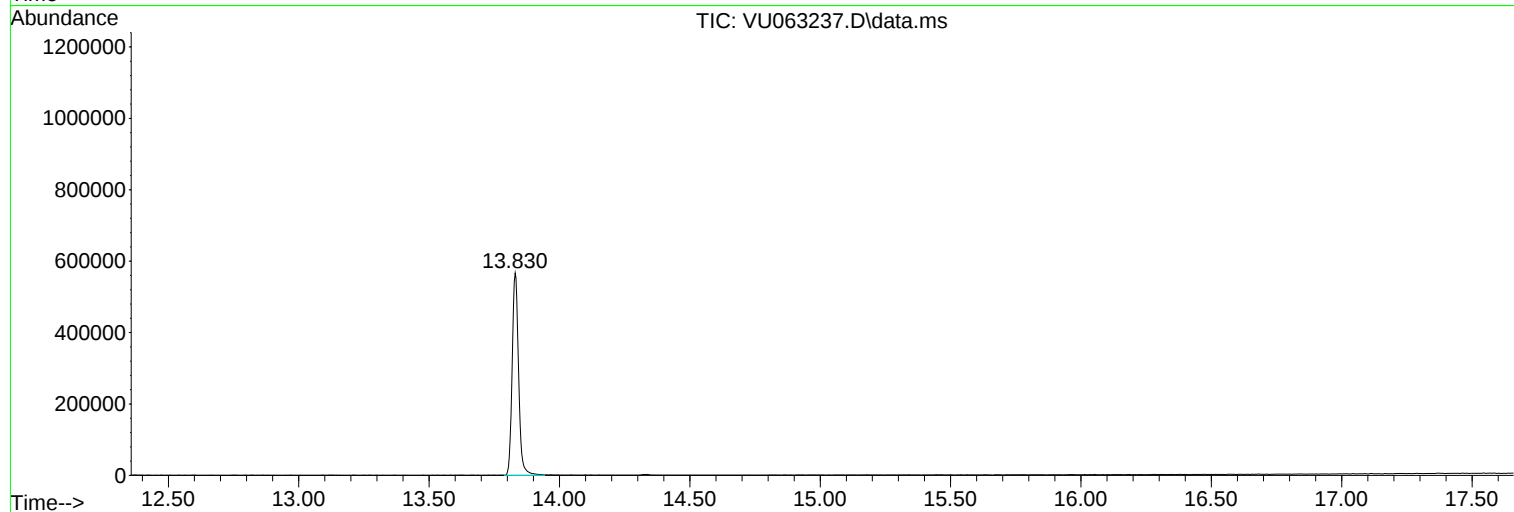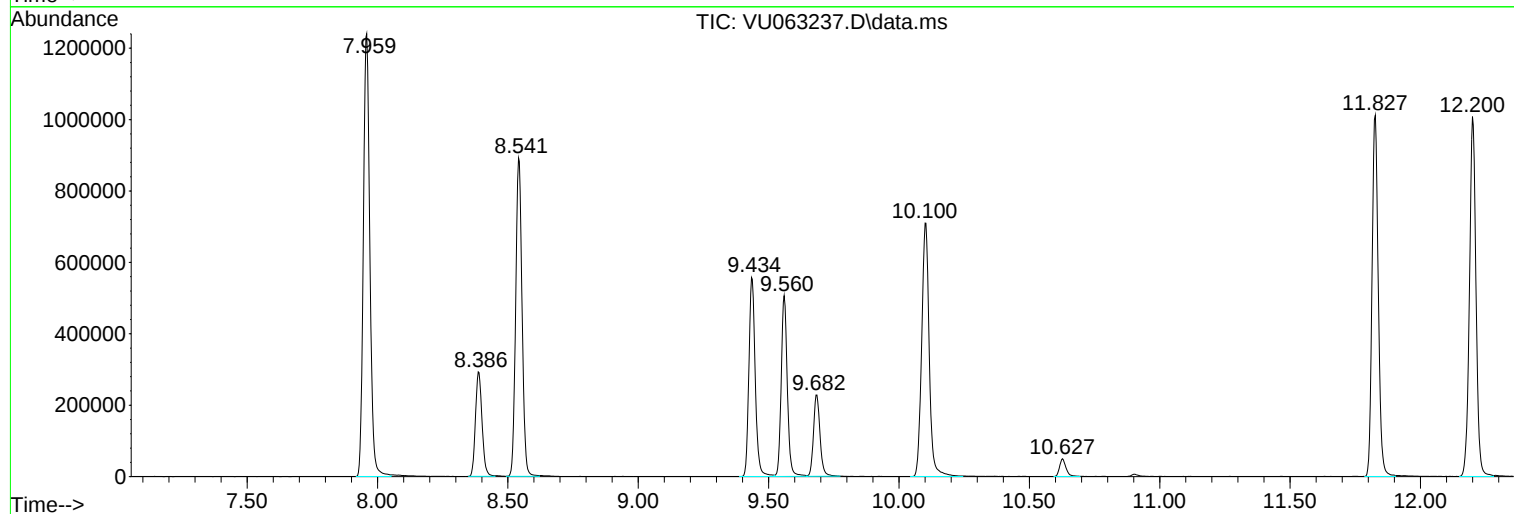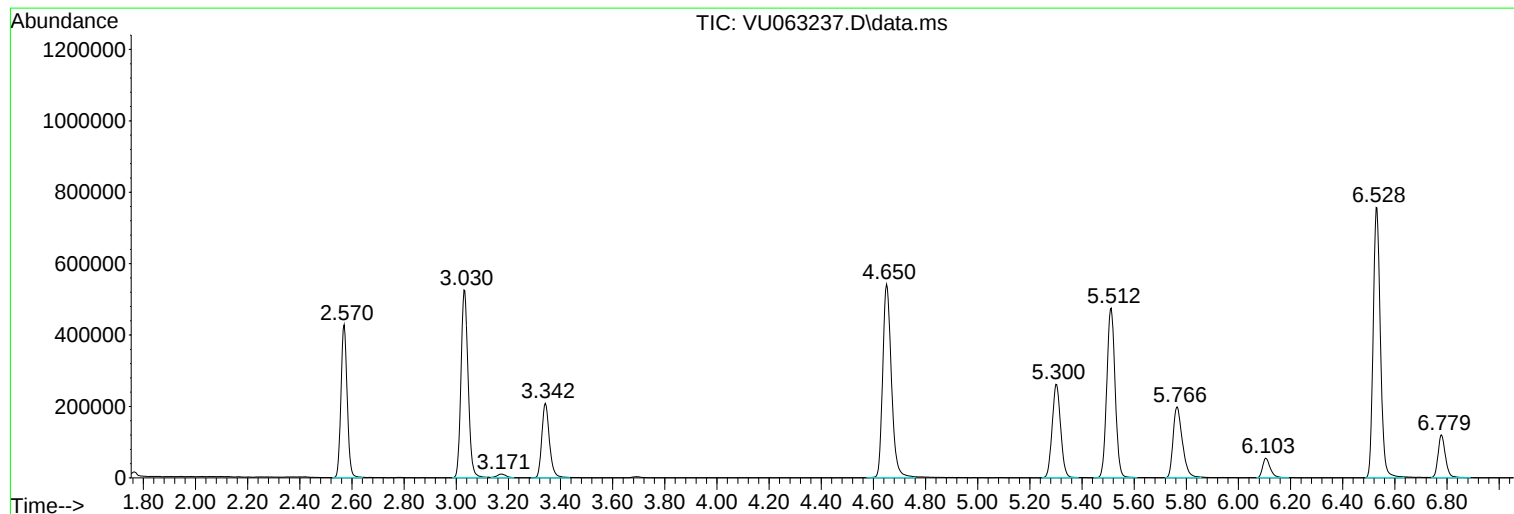

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
Data File : VU063237.D
Acq On : 11 Feb 2025 15:45
Operator : MD/SY
Sample : Q1172-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
Data File : VU063237.D
Acq On : 11 Feb 2025 15:45
Operator : MD/SY
Sample : Q1172-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-RVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------