

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
 Data File : VU063239.D
 Acq On : 11 Feb 2025 16:36
 Operator : MD/SY
 Sample : Q1172-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 PT-UNRVOA-WS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063239.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.129	250	261	284	rVB	638784	943874	29.86%	3.053%
2	3.033	530	542	562	rBV	27561	53016	1.68%	0.171%
3	3.348	621	640	674	rBV	1264868	2901989	91.82%	9.387%
4	3.853	780	797	830	rBV	290861	694050	21.96%	2.245%
5	4.647	1023	1044	1066	rBV	88968	228951	7.24%	0.741%
6	4.959	1126	1141	1174	rBV	403221	906173	28.67%	2.931%
7	5.515	1298	1314	1341	rBV2	210969	444175	14.05%	1.437%
8	6.107	1482	1498	1525	rBV	53953	115794	3.66%	0.375%
9	6.907	1734	1747	1780	rBV	246006	477008	15.09%	1.543%
10	7.595	1947	1961	1996	rBV	664373	1186769	37.55%	3.839%
11	8.200	2136	2149	2174	rBV	466605	816875	25.85%	2.642%
12	8.563	2249	2262	2286	rBV	438814	764012	24.17%	2.471%
13	9.521	2547	2560	2574	rBV	175391	294685	9.32%	0.953%
14	10.473	2844	2856	2887	rBV	593178	934538	29.57%	3.023%
15	10.624	2894	2903	2919	rBV	53129	84678	2.68%	0.274%
16	10.769	2935	2948	2957	rBV	1146117	1912897	60.52%	6.188%
17	10.894	2975	2987	3002	rBV	982869	1503707	47.58%	4.864%
18	10.975	3002	3012	3030	rVV	376586	612336	19.37%	1.981%
19	11.081	3030	3045	3072	rVB2	1424111	2503514	79.21%	8.098%
20	11.409	3132	3147	3154	rBV	704038	1110974	35.15%	3.594%
21	11.457	3154	3162	3186	rVB	1532446	2368414	74.94%	7.661%
22	11.630	3197	3216	3237	rBV	2028550	3160513	100.00%	10.224%
23	11.737	3237	3249	3256	rBV	349756	573213	18.14%	1.854%
24	11.782	3256	3263	3276	rVB	351022	543388	17.19%	1.758%
25	12.196	3377	3392	3424	rBV	1428652	2259902	71.50%	7.310%
26	13.836	3885	3902	3918	rBV6	19383	36651	1.16%	0.119%
27	14.010	3943	3956	3968	rBV	819712	1274076	40.31%	4.121%
28	14.077	3968	3977	4001	rVB	148642	249878	7.91%	0.808%
29	14.318	4039	4052	4081	rBV	1189790	1957662	61.94%	6.333%




Sum of corrected areas: 30913712

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
Data File : VU063239.D
Acq On : 11 Feb 2025 16:36
Operator : MD/SY
Sample : Q1172-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

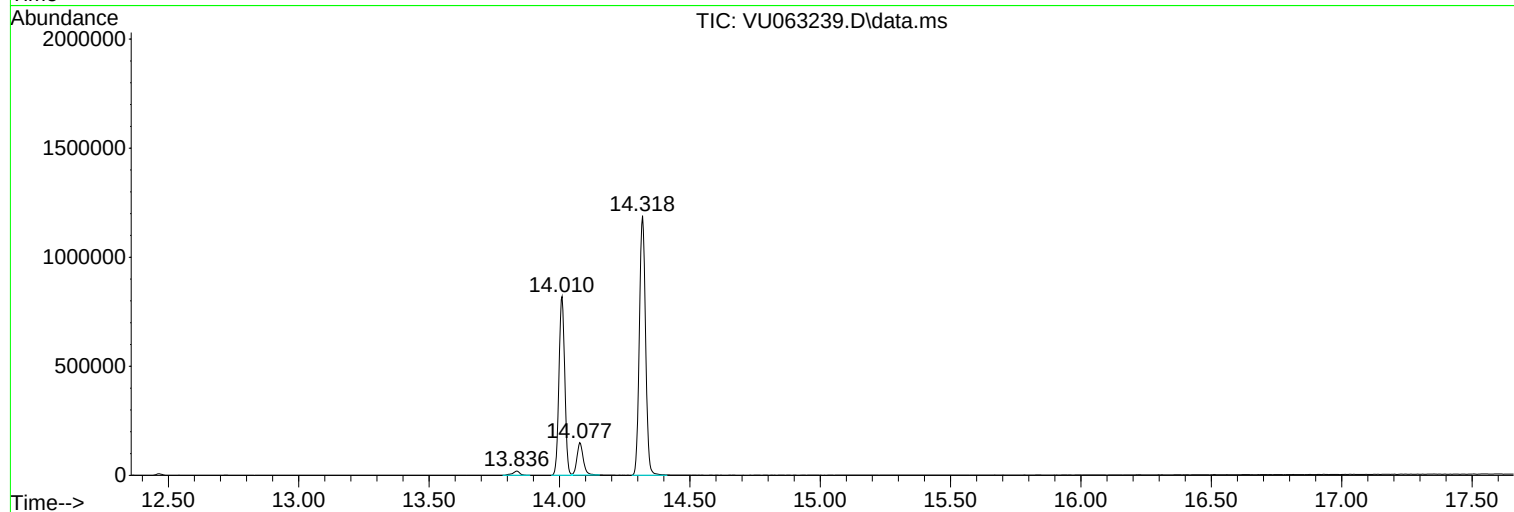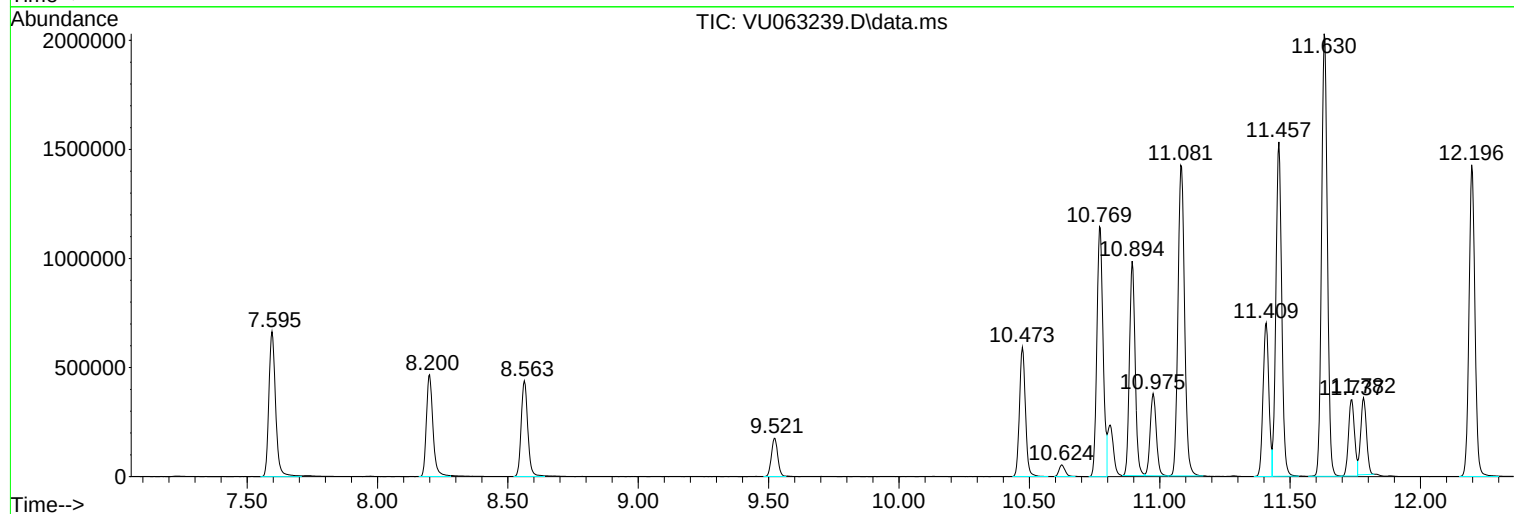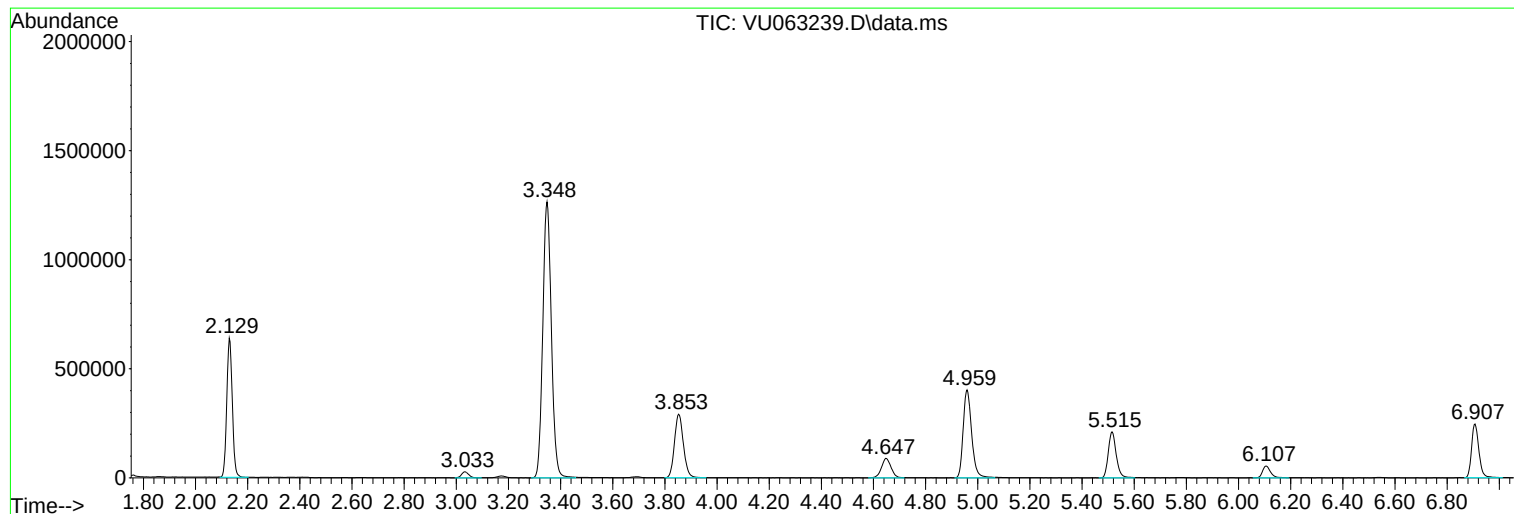

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
Data File : VU063239.D
Acq On : 11 Feb 2025 16:36
Operator : MD/SY
Sample : Q1172-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
Data File : VU063239.D
Acq On : 11 Feb 2025 16:36
Operator : MD/SY
Sample : Q1172-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
PT-UNRVOA-WS

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------