

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
 Data File : VU063241.D
 Acq On : 11 Feb 2025 17:26
 Operator : MD/SY
 Sample : VIBLK
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063241.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.129	258	261	267	rVB4	1212	1158	1.09%	0.297%
2	3.036	535	543	551	rBV5	1327	2355	2.23%	0.605%
3	3.174	570	586	603	rVB	10129	24085	22.77%	6.187%
4	3.692	732	747	758	rBV7	2723	6462	6.11%	1.660%
5	4.621	1020	1036	1052	rBV4	2064	6479	6.13%	1.664%
6	6.107	1485	1498	1524	rBV	52003	105768	100.00%	27.169%
7	10.631	2894	2905	2929	rBV	33808	62460	59.05%	16.044%
8	10.785	2942	2953	2963	rBV6	2655	5116	4.84%	1.314%
9	10.907	2979	2991	3007	rVB3	2133	4507	4.26%	1.158%
10	11.090	3040	3048	3050	rBV2	1458	1379	1.30%	0.354%
11	11.466	3156	3165	3178	rBV3	2450	4817	4.55%	1.237%
12	11.637	3209	3218	3234	rVB2	4238	6825	6.45%	1.753%
13	11.756	3250	3255	3260	rBV4	1231	1615	1.53%	0.415%
14	12.190	3378	3390	3415	rBV3	45818	98774	93.39%	25.373%
15	13.855	3900	3908	3918	rVB4	1519	2256	2.13%	0.580%
16	14.010	3950	3956	3966	rVB6	6121	8063	7.62%	2.071%
17	14.103	3975	3985	3989	rBV3	2877	4422	4.18%	1.136%
18	14.325	4042	4054	4069	rBV3	24356	42753	40.42%	10.982%




Sum of corrected areas: 389294

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
Data File : VU063241.D
Acq On : 11 Feb 2025 17:26
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

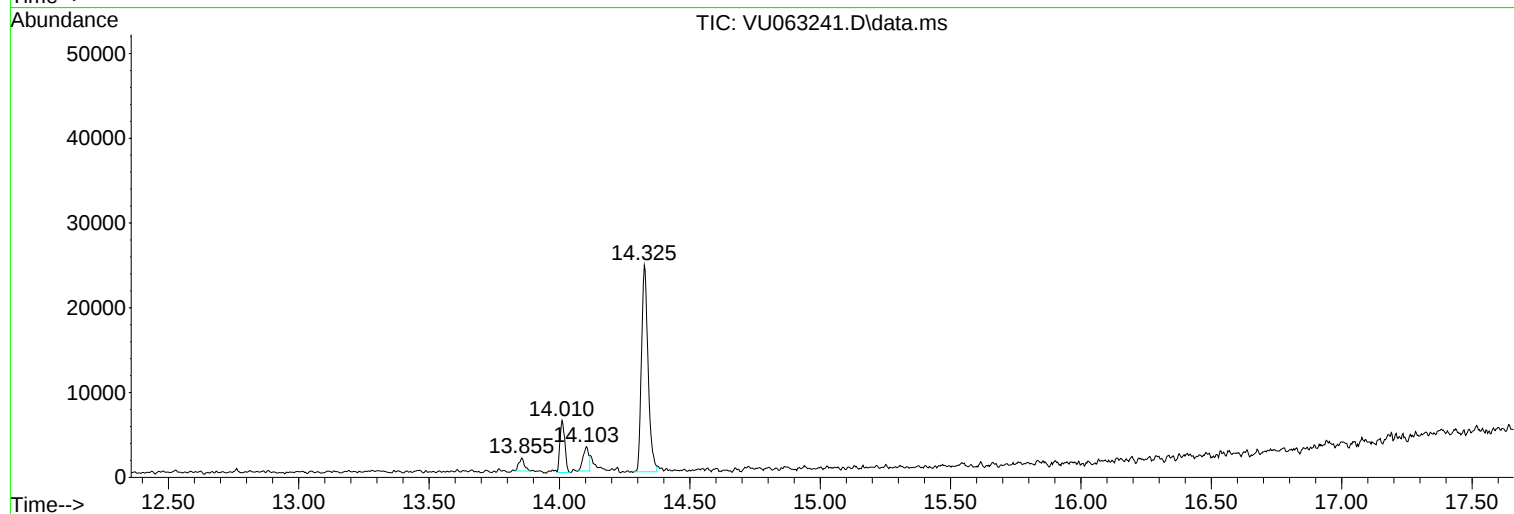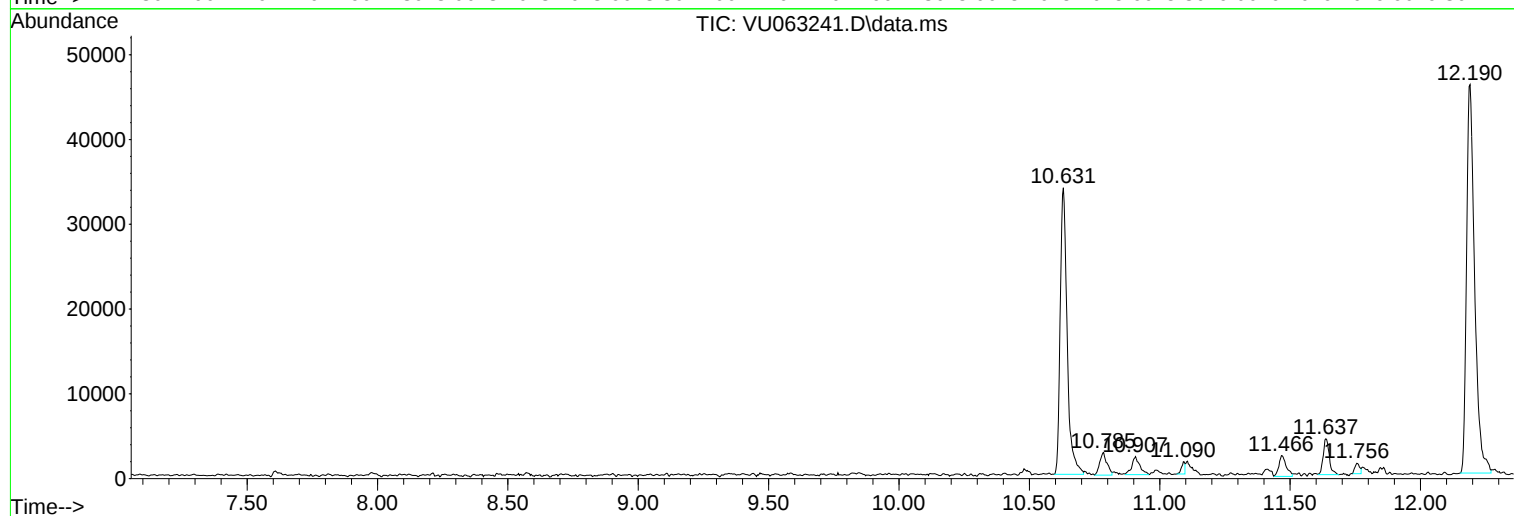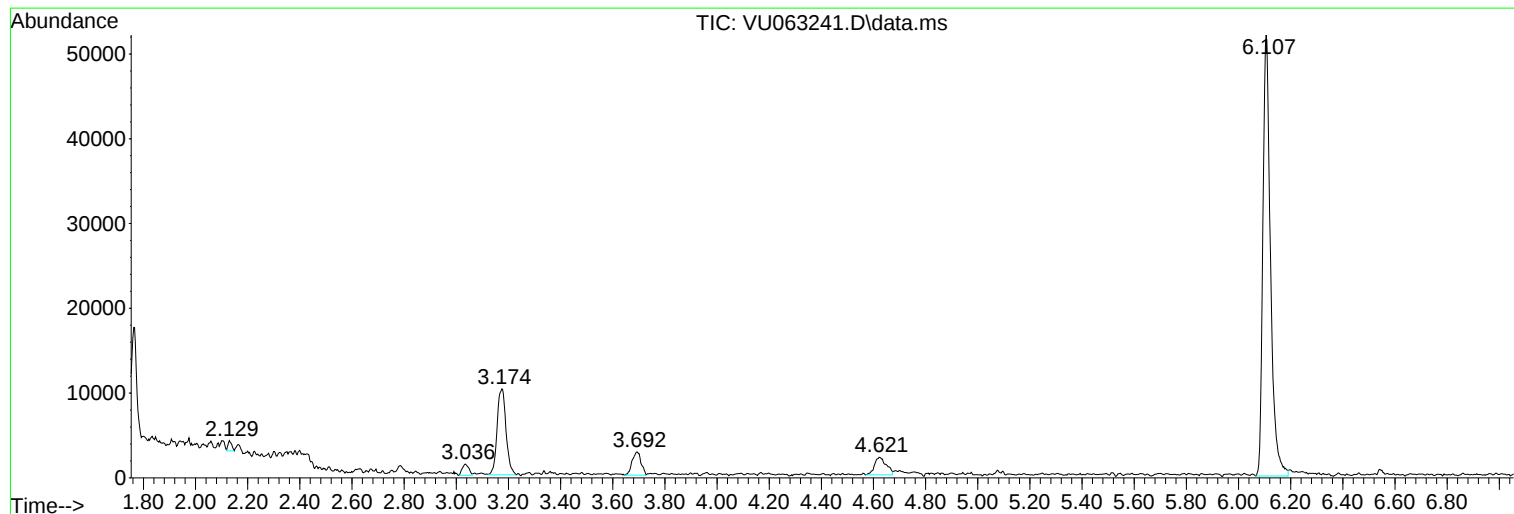

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
Data File : VU063241.D
Acq On : 11 Feb 2025 17:26
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021125\
Data File : VU063241.D
Acq On : 11 Feb 2025 17:26
Operator : MD/SY
Sample : VIBLK
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------