

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021225\
 Data File : VU063250.D
 Acq On : 12 Feb 2025 12:17
 Operator : MD/SY
 Sample : VU0212WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0212WBL01

Quant Time: Feb 13 03:10:06 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Feb 11 08:42:19 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.107	96	47954	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.627	95	12922	0.817	ug/l	0.00
Spiked Amount 1.000			Recovery	=	82.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	12781	0.777	ug/l	0.00
Spiked Amount 1.000			Recovery	=	78.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021225\
Data File : VU063250.D
Acq On : 12 Feb 2025 12:17
Operator : MD/SY
Sample : VU0212WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0212WBL01

Quant Time: Feb 13 03:10:06 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Feb 11 08:42:19 2025
Response via : Initial Calibration




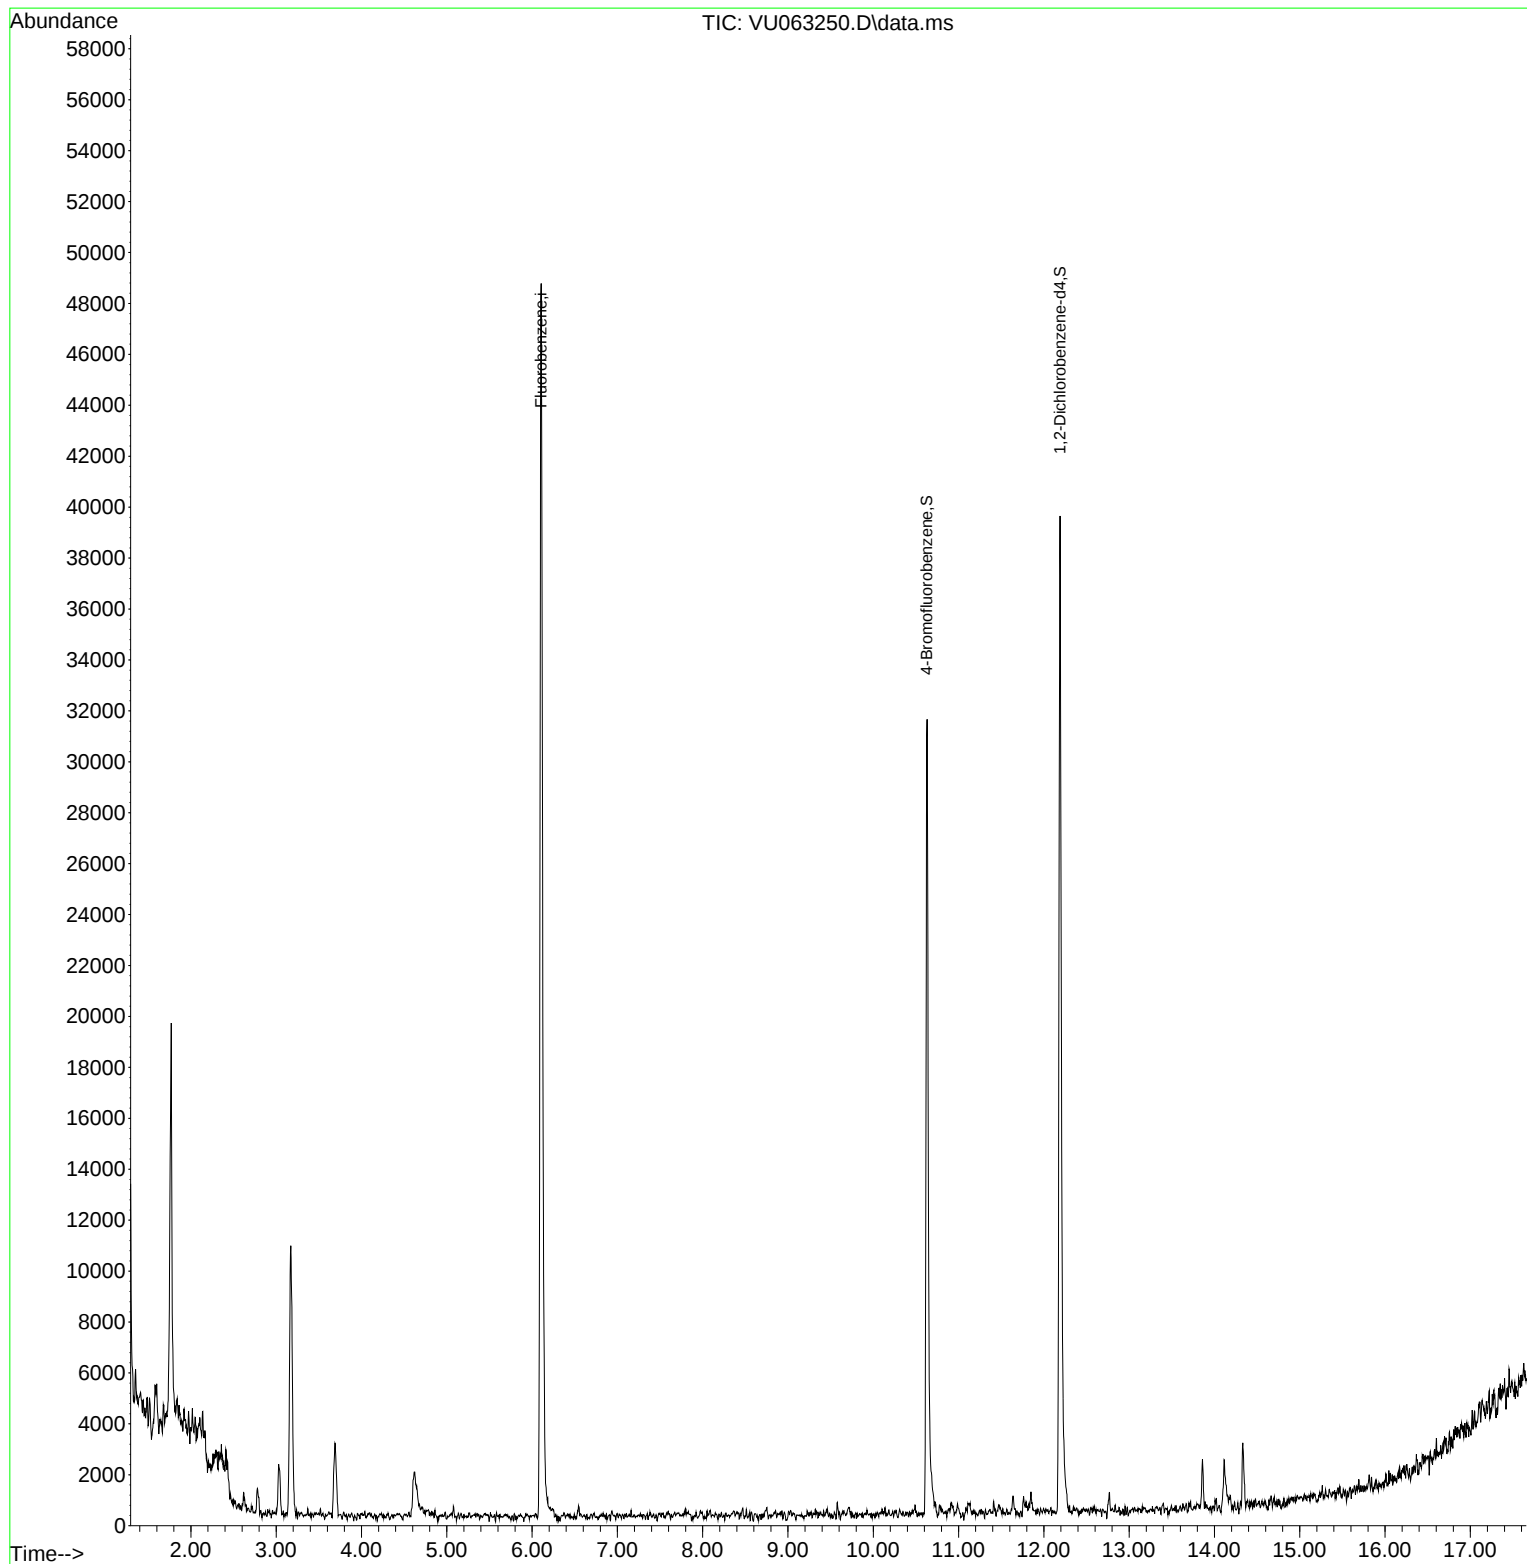


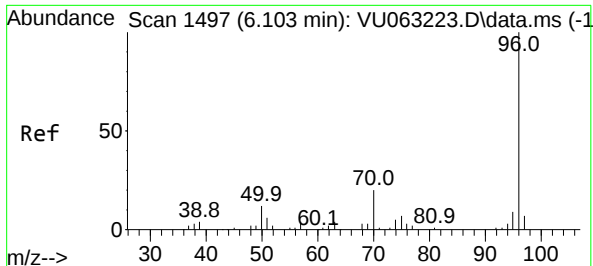

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.107 min Scan# 1497
Delta R.T. 0.004 min
Lab File: VU063250.D
Acq: 12 Feb 2025 12:17




Instrument :
MSVOA_U
ClientSampleId :
VU0212WBL01


Tgt Ion: 96	Resp: 47954
Ion Ratio	Lower Upper
96 100	
70 20.6	15.6 23.4
95 9.6	7.3 10.9
97 6.5	0.0 0.0#

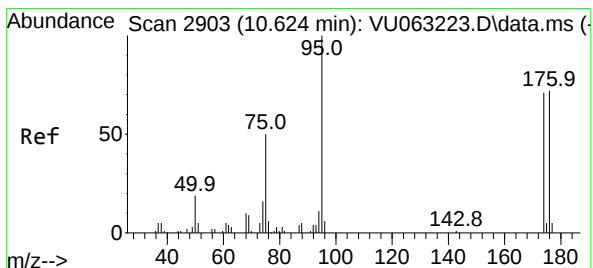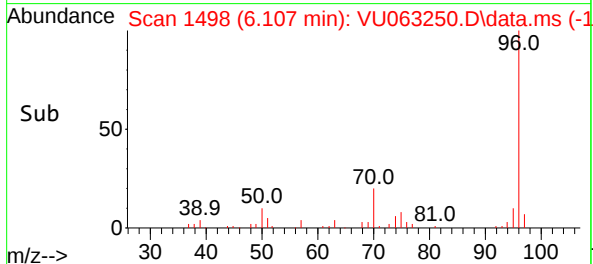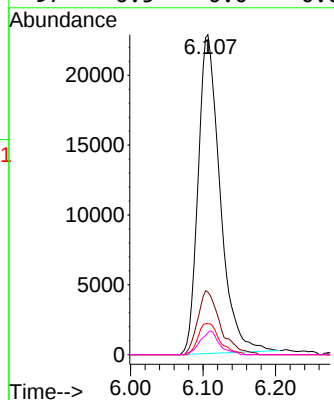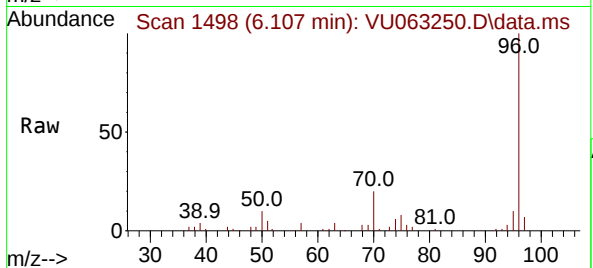

#57
4-Bromofluorobenzene
Concen: 0.817 ug/l
RT: 10.627 min Scan# 2904
Delta R.T. 0.003 min
Lab File: VU063250.D
Acq: 12 Feb 2025 12:17

Tgt Ion: 95	Resp: 12922
Ion Ratio	Lower Upper
95 100	
174 82.6	58.6 88.0
176 72.7	58.2 87.4

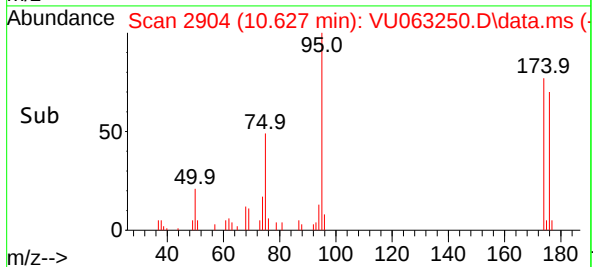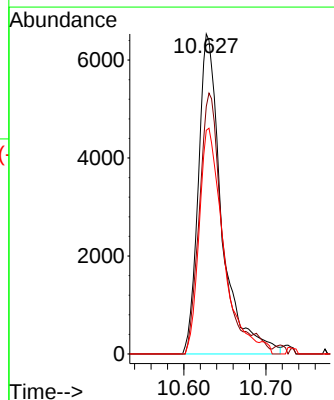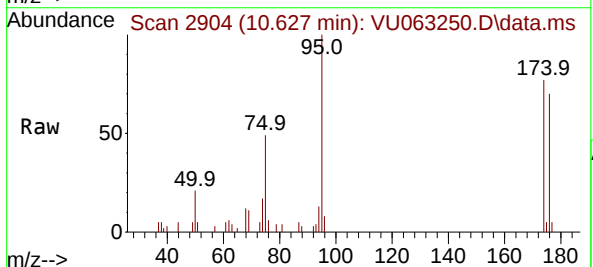

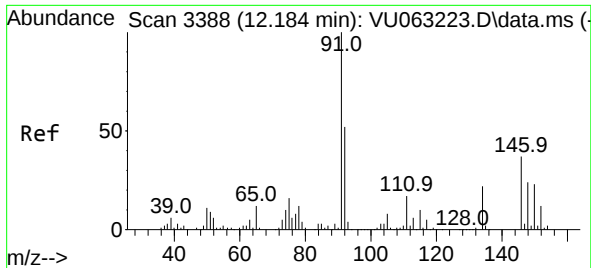

#68

1,2-Dichlorobenzene-d4

Concen: 0.777 ug/l

RT: 12.190 min Scan# 31

Delta R.T. 0.006 min

Lab File: VU063250.D


Acq: 12 Feb 2025 12:17

Instrument :

MSVOA_U

ClientSampleId :

VU0212WBL01

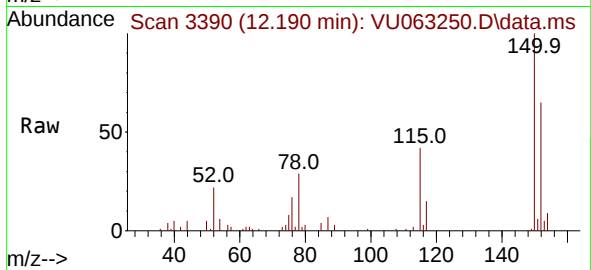

Tgt Ion:152 Resp: 12781

Ion Ratio Lower Upper

152 100

115 60.8 0.0 275.2

150 158.5 0.0 658.4

