

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021225\
 Data File : VU063250.D
 Acq On : 12 Feb 2025 12:17
 Operator : MD/SY
 Sample : VU0212WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0212WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063250.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.769	147	149	163	rVB	15302	13649	13.42%	4.461%
2	2.428	352	354	363	rVB3	1485	1621	1.59%	0.530%
3	2.779	458	463	467	rBV3	869	1041	1.02%	0.340%
4	3.030	533	541	552	rVB4	1976	3554	3.49%	1.162%
5	3.171	573	585	603	rVB2	10605	23785	23.39%	7.774%
6	3.689	736	746	758	rBV7	2894	6373	6.27%	2.083%
7	4.621	1023	1036	1041	rBV2	1764	4029	3.96%	1.317%
8	6.107	1484	1498	1520	rBV	48508	101698	100.00%	33.241%
9	10.631	2894	2905	2931	rBV2	31215	58974	57.99%	19.276%
10	12.190	3376	3390	3421	rBV	39176	78755	77.44%	25.742%
11	12.769	3560	3570	3574	rBV2	1012	1557	1.53%	0.509%
12	13.859	3902	3909	3916	rVB5	1947	2528	2.49%	0.826%
13	14.113	3977	3988	4000	rBV7	2076	4570	4.49%	1.494%
14	14.331	4051	4056	4067	rVB3	2564	3811	3.75%	1.246%




Sum of corrected areas: 305945

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021225\
Data File : VU063250.D
Acq On : 12 Feb 2025 12:17
Operator : MD/SY
Sample : VU0212WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0212WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

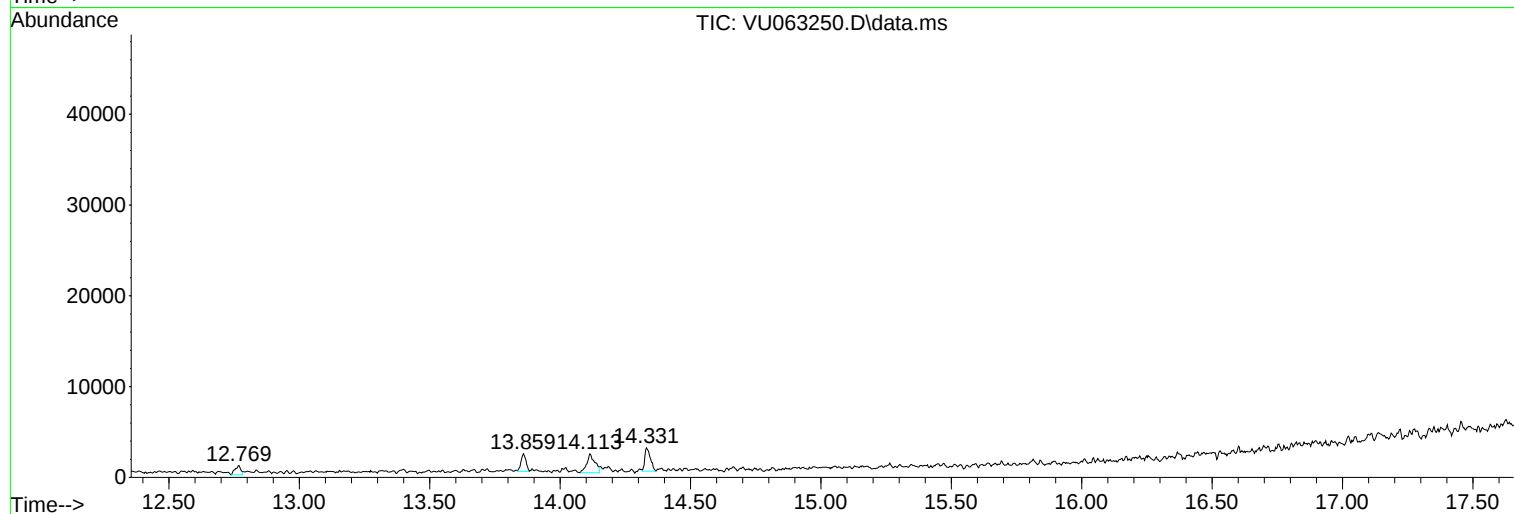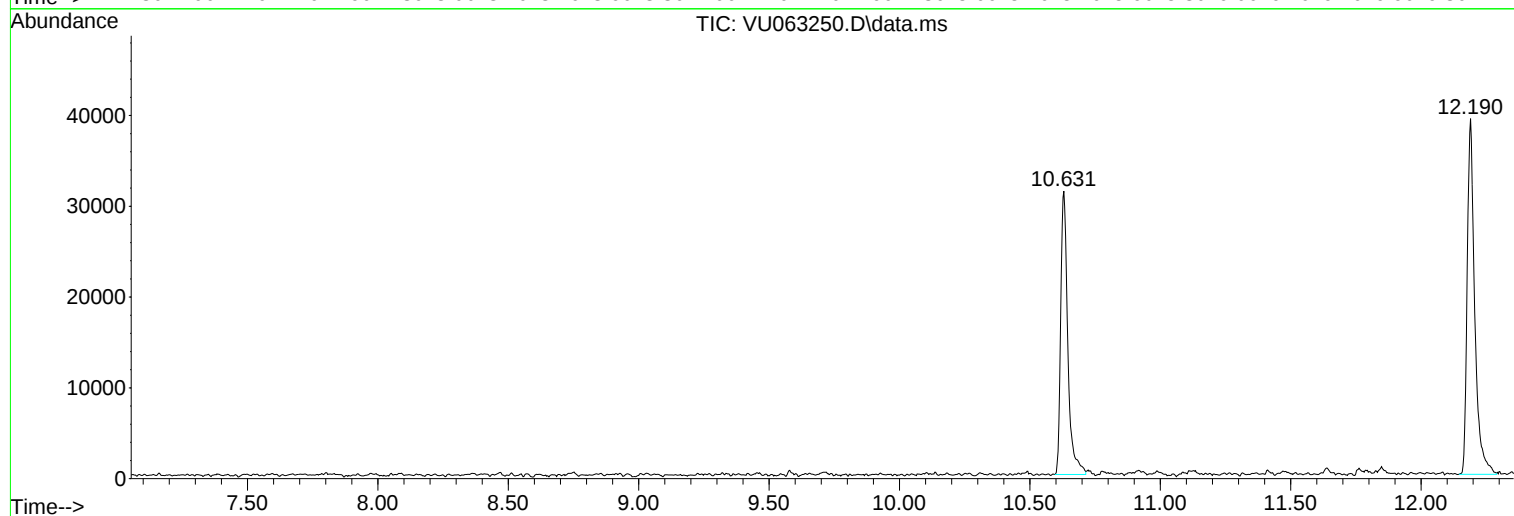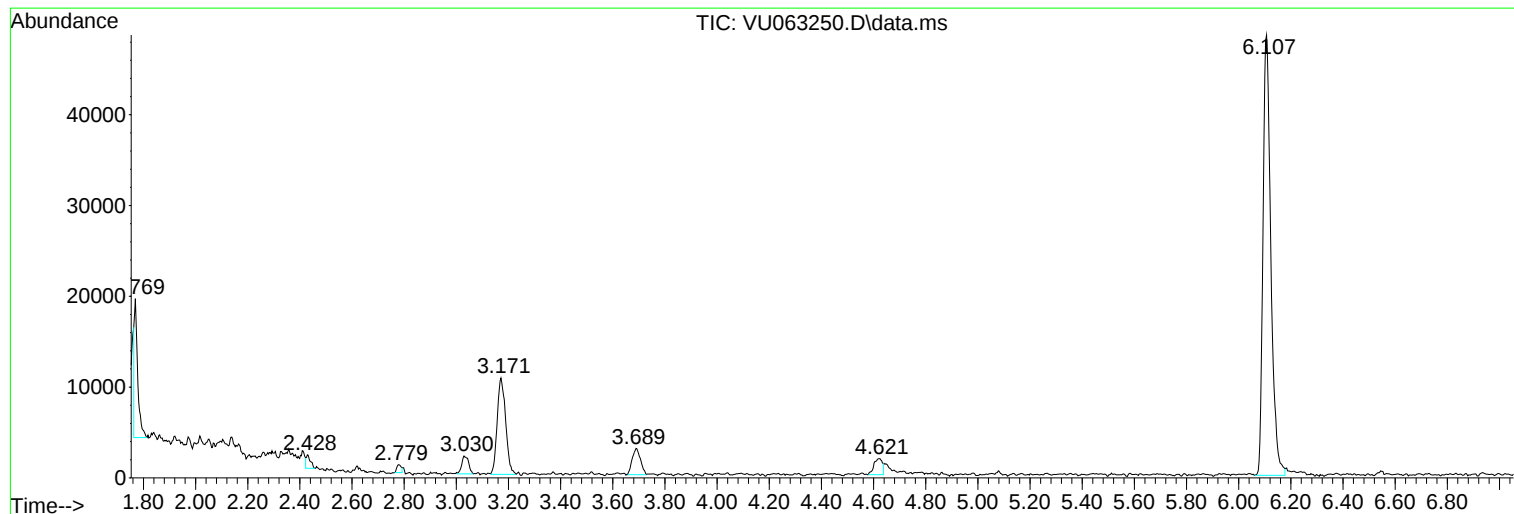

Library Search Compound Report

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021225\
Data File : VU063250.D
Acq On : 12 Feb 2025 12:17
Operator : MD/SY
Sample : VU0212WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0212WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021225\
Data File : VU063250.D
Acq On : 12 Feb 2025 12:17
Operator : MD/SY
Sample : VU0212WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0212WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------