


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021225\
Data File : VU063248.D
Acq On : 12 Feb 2025 10:13
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Feb 11 08:42:19 2025

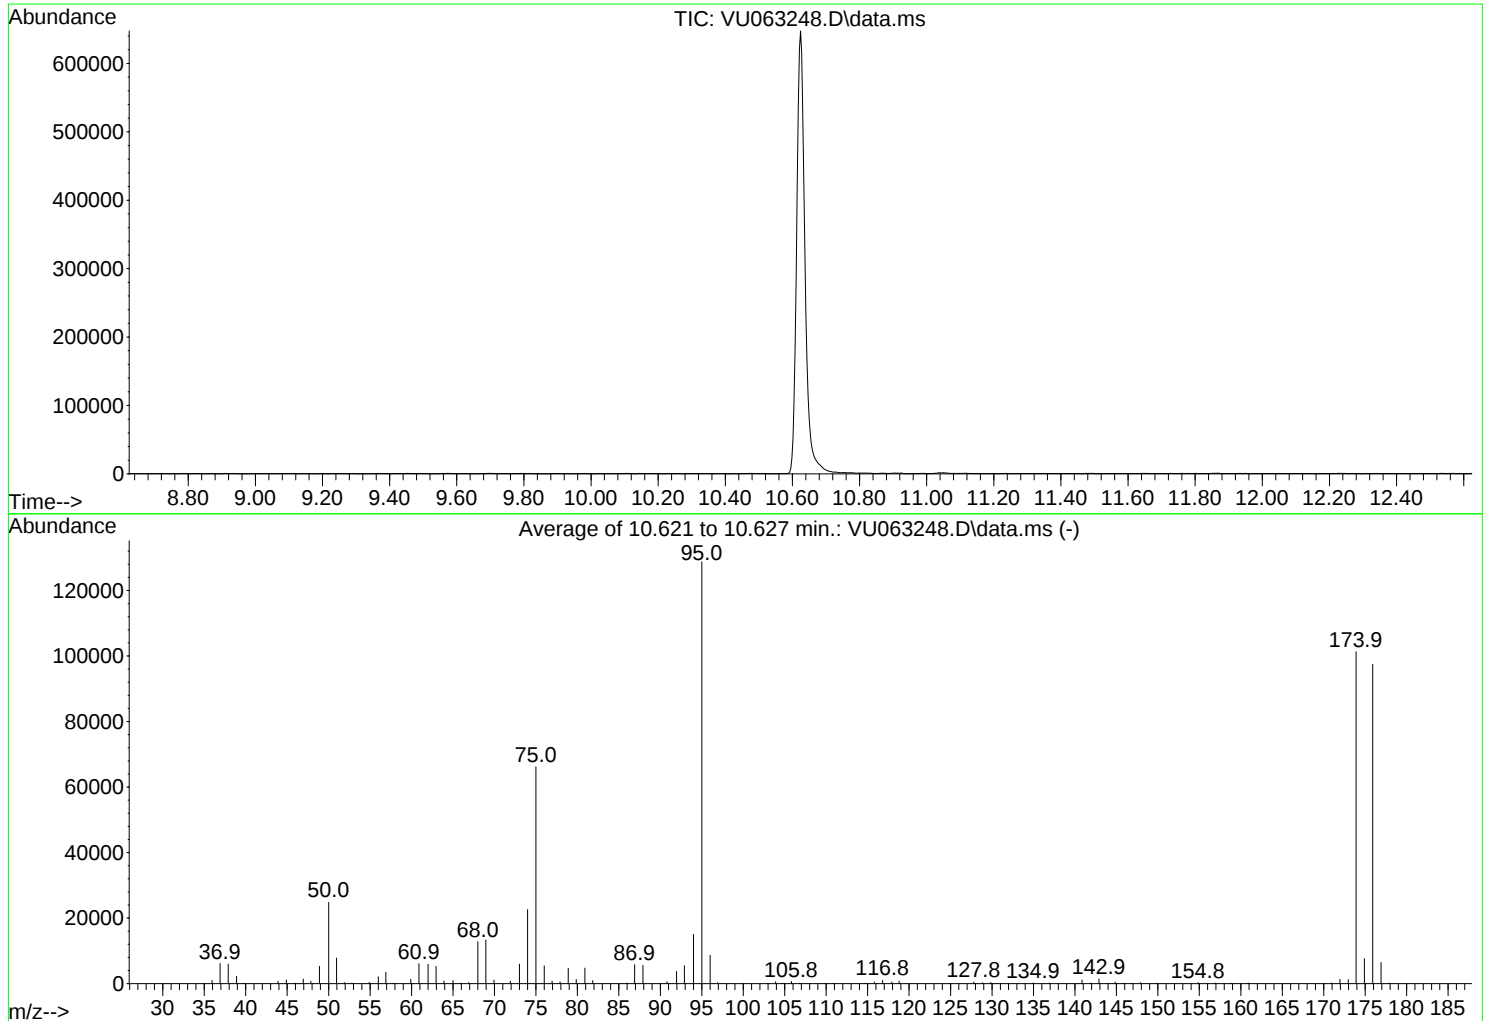

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	24832	PASS
75	95	30	60	51.4	66152	PASS
95	95	100	100	100.0	128739	PASS
96	95	5	9	6.7	8666	PASS
173	174	0.00	2	1.2	1241	PASS
174	95	50	100	78.7	101285	PASS
175	174	5	9	7.5	7621	PASS
176	174	95	101	96.2	97483	PASS
177	176	5	9	6.6	6463	PASS