

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021325\
 Data File : VU063263.D
 Acq On : 13 Feb 2025 13:05
 Operator : MD/SY
 Sample : VU0213WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0213WBL01

Quant Time: Feb 14 04:44:02 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
 Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
 QLast Update : Tue Feb 11 08:42:19 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Fluorobenzene	6.107	96	46092	1.000	ug/l	# 0.00
System Monitoring Compounds						
57) 4-Bromofluorobenzene	10.627	95	13151	0.865	ug/l	0.00
Spiked Amount 1.000			Recovery	=	86.000%	
68) 1,2-Dichlorobenzene-d4	12.190	152	12766	0.807	ug/l	0.00
Spiked Amount 1.000			Recovery	=	81.000%	


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021325\
Data File : VU063263.D
Acq On : 13 Feb 2025 13:05
Operator : MD/SY
Sample : VU0213WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0213WBL01

Quant Time: Feb 14 04:44:02 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER
QLast Update : Tue Feb 11 08:42:19 2025
Response via : Initial Calibration




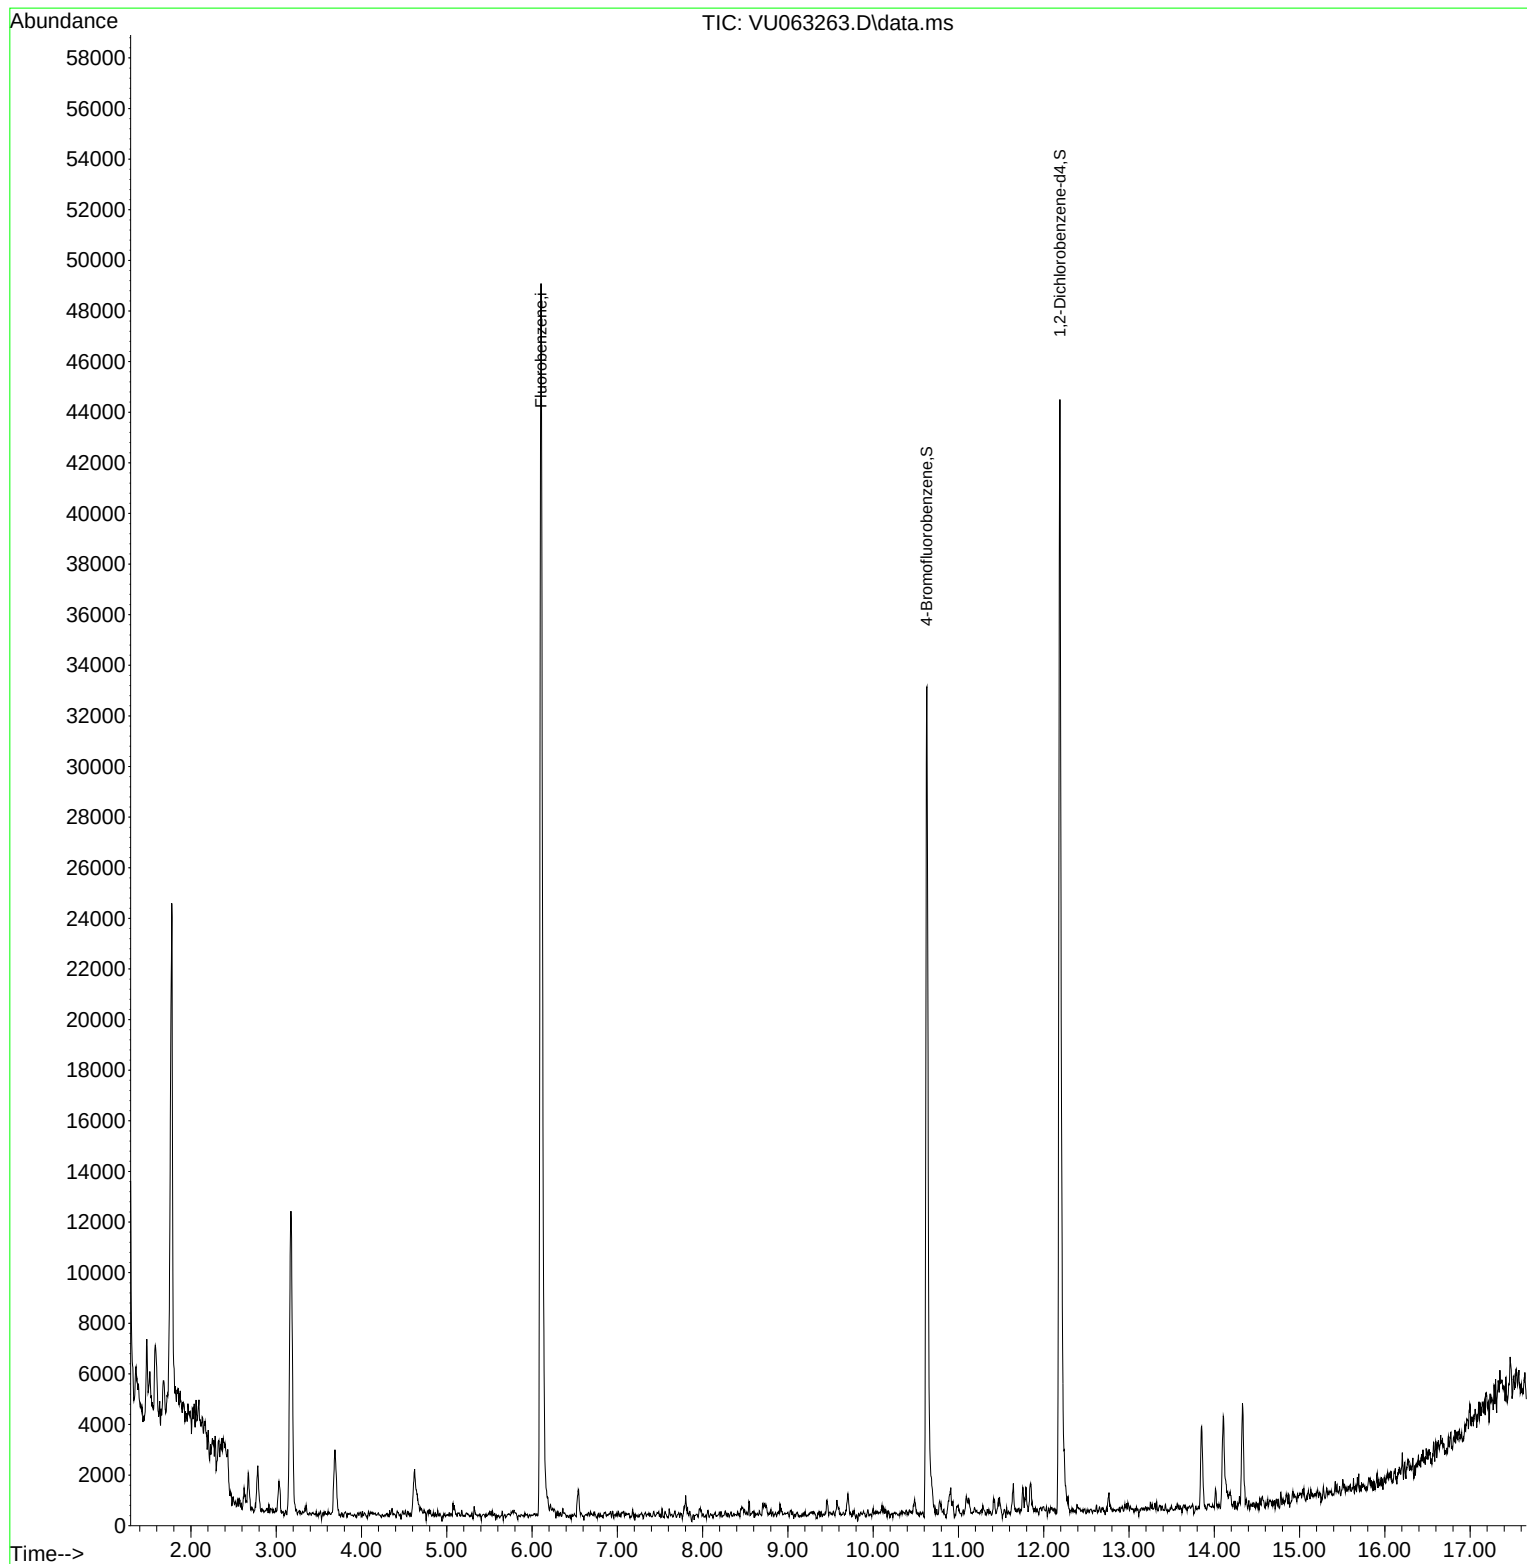


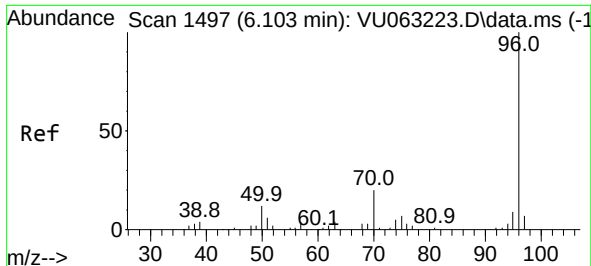

#1
Fluorobenzene
Concen: 1.000 ug/l
RT: 6.107 min Scan# 1497
Delta R.T. 0.004 min
Lab File: VU063263.D
Acq: 13 Feb 2025 13:05




Instrument :
MSVOA_U
ClientSampleId :
VU0213WBL01


Tgt Ion: 96	Resp: 46092
Ion Ratio	Lower Upper
96 100	
70 19.5	15.6 23.4
95 8.0	7.3 10.9
97 6.8	0.0 0.0

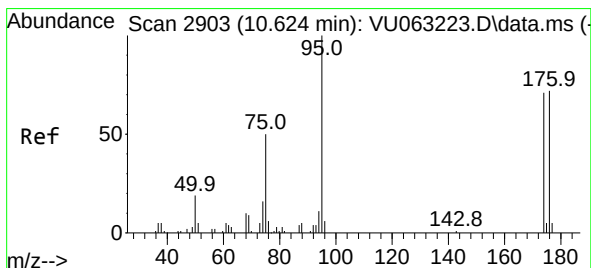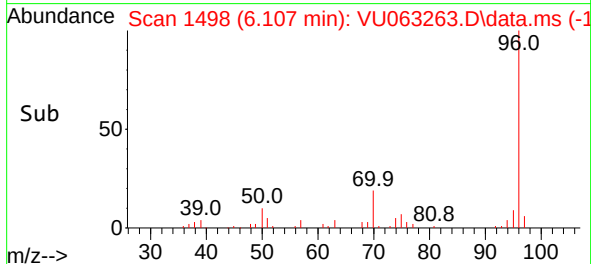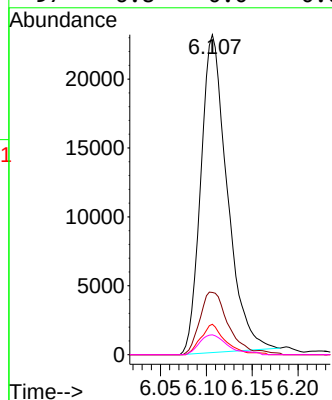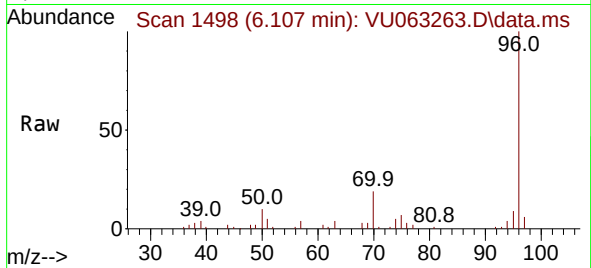

#57
4-Bromofluorobenzene
Concen: 0.865 ug/l
RT: 10.627 min Scan# 2904
Delta R.T. 0.003 min
Lab File: VU063263.D
Acq: 13 Feb 2025 13:05


Tgt Ion: 95	Resp: 13151
Ion Ratio	Lower Upper
95 100	
174 80.3	58.6 88.0
176 79.7	58.2 87.4

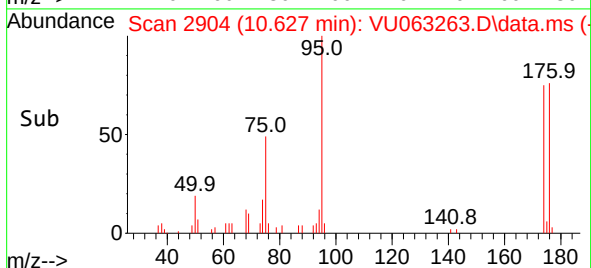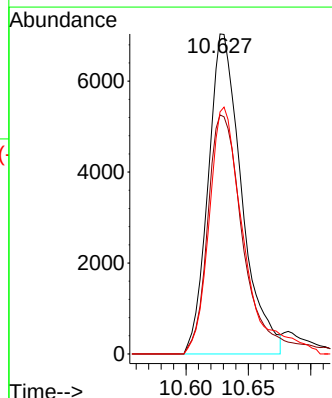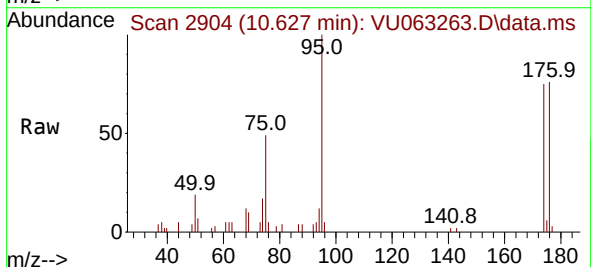

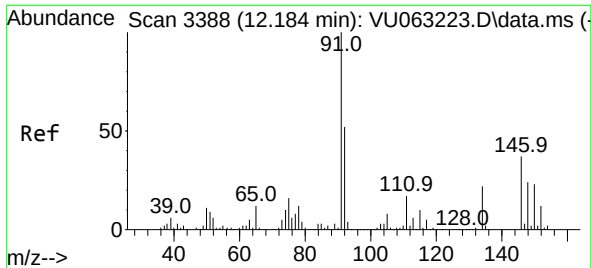

#68
 1,2-Dichlorobenzene-d4
 Concen: 0.807 ug/l
 RT: 12.190 min Scan# 31
 Delta R.T. 0.006 min
 Lab File: VU063263.D
 Acq: 13 Feb 2025 13:05

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0213WBL01

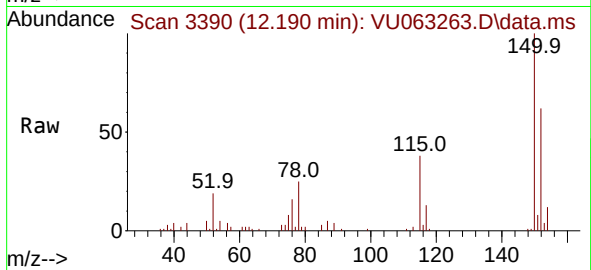

Tgt Ion:	152	Resp:	12766
Ion Ratio	Lower	Upper	
152	100		
115	67.9	0.0	275.2
150	166.4	0.0	658.4

