

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021325\
 Data File : VU063263.D
 Acq On : 13 Feb 2025 13:05
 Operator : MD/SY
 Sample : VU0213WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VU0213WBL01

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M

Title : METHOD 524.2 VOLATILES DRINKING WATER

Signal : TIC: VU063263.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.776	146	151	162	rVB4	19363	25975	26.04%	7.355%
2	2.203	280	284	289	rVB4	1193	1053	1.06%	0.298%
3	2.284	306	309	313	rVB5	1380	1165	1.17%	0.330%
4	2.322	313	321	322	rBV6	1164	1140	1.14%	0.323%
5	2.673	425	430	440	rVB6	1481	2102	2.11%	0.595%
6	2.785	457	465	477	rVB2	1815	3022	3.03%	0.856%
7	3.033	534	542	550	rVB4	1254	2067	2.07%	0.585%
8	3.174	571	586	603	rBV	11991	27450	27.52%	7.773%
9	3.689	737	746	758	rBV5	2471	4939	4.95%	1.399%
10	4.624	1024	1037	1047	rBV	1875	4459	4.47%	1.263%
11	6.107	1486	1498	1528	rBV	48696	99754	100.00%	28.247%
12	6.547	1626	1635	1641	rBV4	1043	1745	1.75%	0.494%
13	9.704	2611	2617	2624	rVB3	812	1094	1.10%	0.310%
14	10.630	2895	2905	2929	rBV2	32829	61847	62.00%	17.513%
15	10.910	2985	2992	2995	rVV3	1198	1755	1.76%	0.497%
16	11.483	3167	3170	3180	rVB3	829	1134	1.14%	0.321%
17	11.643	3210	3220	3229	rBV3	1229	1815	1.82%	0.514%
18	11.756	3249	3255	3260	rBV4	931	1032	1.03%	0.292%
19	11.791	3260	3266	3274	rVB2	983	1351	1.35%	0.383%
20	11.849	3274	3284	3288	rBV4	1108	1771	1.78%	0.501%
21	12.190	3378	3390	3418	rBV2	44033	86777	86.99%	24.572%
22	13.852	3898	3907	3918	rBV5	3261	5592	5.61%	1.583%
23	14.106	3975	3986	3998	rBV5	3650	7537	7.56%	2.134%
24	14.331	4048	4056	4066	rVB4	4001	6576	6.59%	1.862%




Sum of corrected areas: 353152

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021325\
Data File : VU063263.D
Acq On : 13 Feb 2025 13:05
Operator : MD/SY
Sample : VU0213WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0213WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

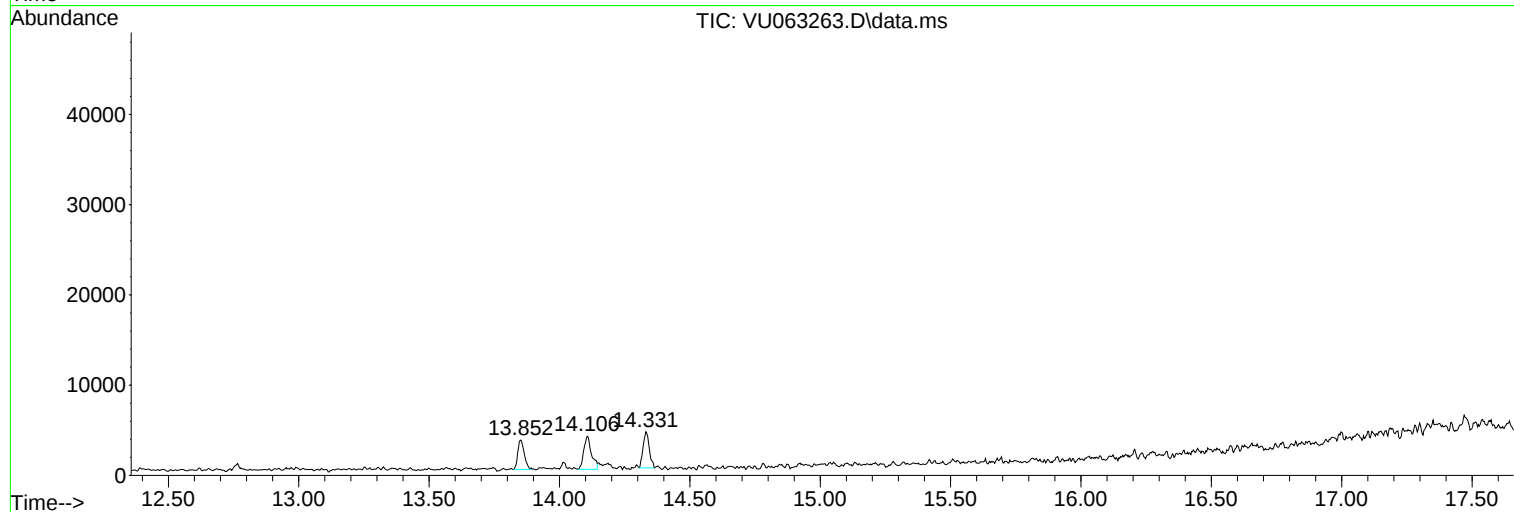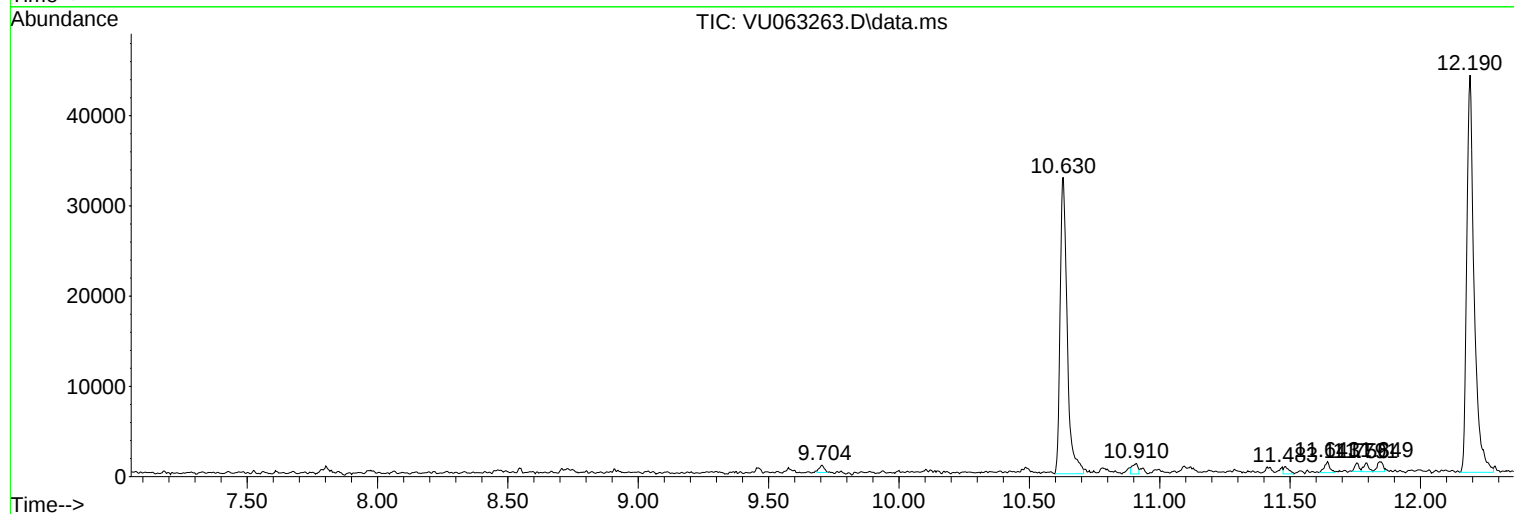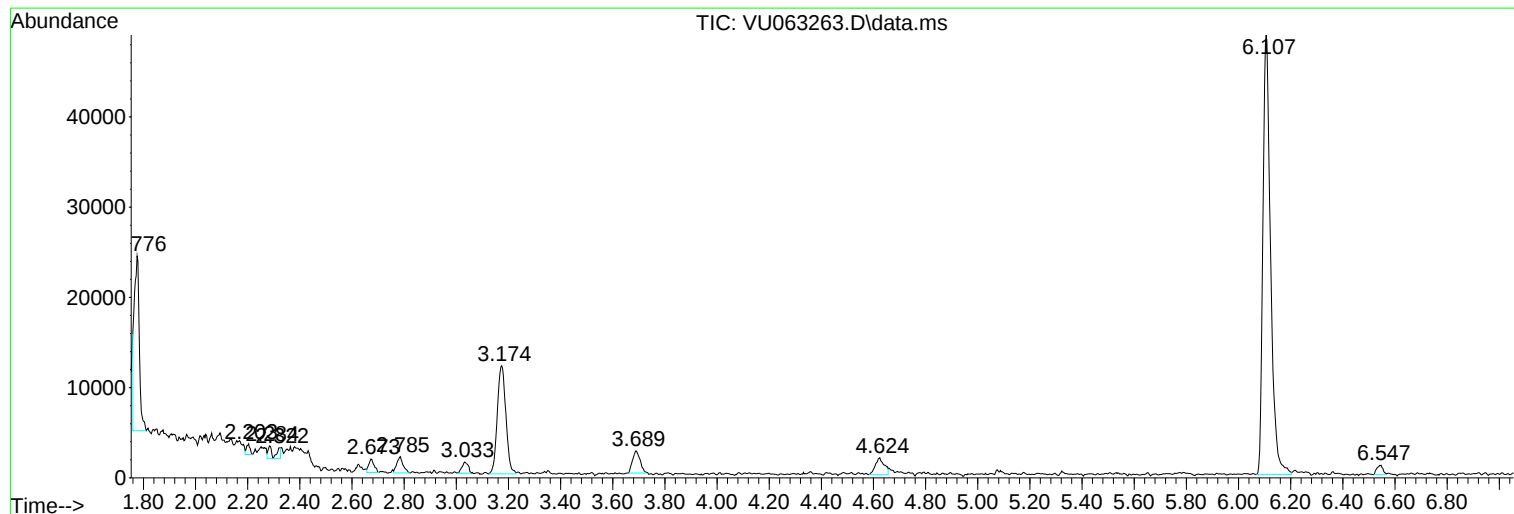

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021325\
Data File : VU063263.D
Acq On : 13 Feb 2025 13:05
Operator : MD/SY
Sample : VU0213WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0213WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021325\
Data File : VU063263.D
Acq On : 13 Feb 2025 13:05
Operator : MD/SY
Sample : VU0213WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VU0213WBL01

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Quant Title : METHOD 524.2 VOLATILES DRINKING WATER

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------