


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021325\
Data File : VU063261.D
Acq On : 13 Feb 2025 08:06
Operator : MD/SY
Sample : BFB
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\524U021025DW.M
Title : METHOD 524.2 VOLATILES DRINKING WATER
Last Update : Tue Feb 11 08:42:19 2025

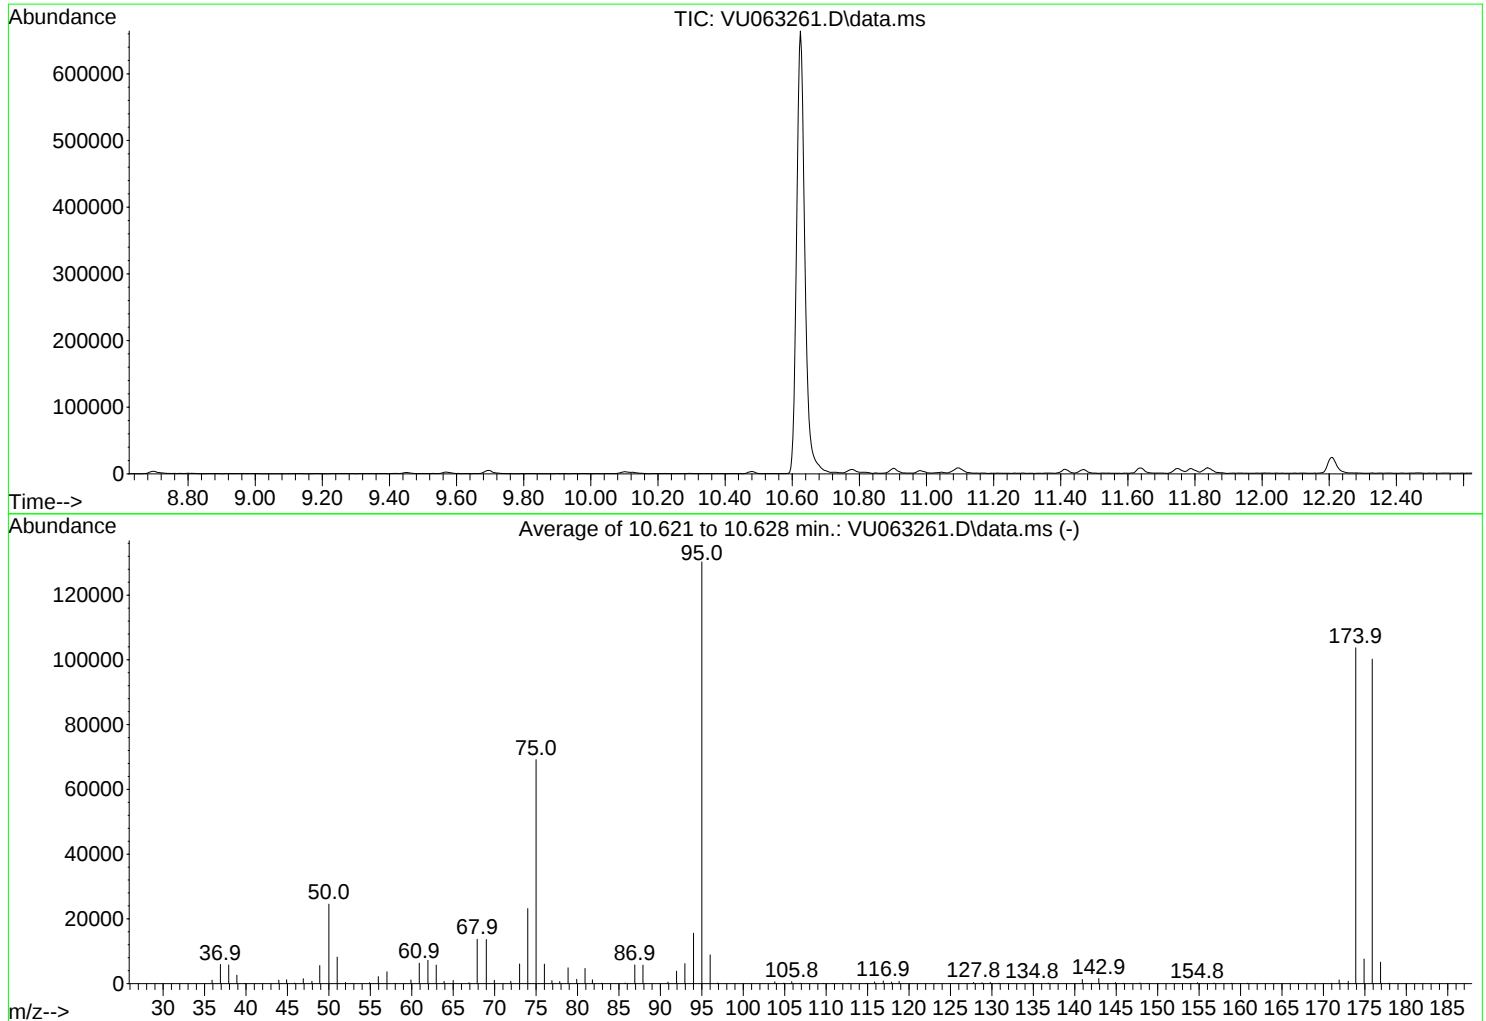

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2888

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	24589	PASS
75	95	30	60	53.1	69179	PASS
95	95	100	100	100.0	130275	PASS
96	95	5	9	6.8	8880	PASS
173	174	0.00	2	0.7	745	PASS
174	95	50	100	79.6	103747	PASS
175	174	5	9	7.4	7635	PASS
176	174	95	101	96.6	100208	PASS
177	176	5	9	6.6	6618	PASS