

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021924\
 Data File : VU057878.D
 Acq On : 19 Feb 2024 11:36
 Operator : MD/SY
 Sample : VU0219WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK040

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

Signal : TIC: VU057878.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	111	rVB	129717	151509	15.81%	2.154%
2	1.888	178	186	201	rVB	95071	131062	13.68%	1.863%
3	2.496	373	375	378	rBV	330	186	0.02%	0.003%
4	2.557	381	394	411	rBV	202154	329789	34.42%	4.689%
5	2.708	439	441	447	rVB2	529	372	0.04%	0.005%
6	2.769	457	460	461	rBV	328	198	0.02%	0.003%
7	2.901	499	501	505	rVB	351	203	0.02%	0.003%
8	2.949	513	516	519	rBV2	362	308	0.03%	0.004%
9	3.033	532	542	555	rVV3	10922	20305	2.12%	0.289%
10	3.168	574	584	585	rBV2	1364	1507	0.16%	0.021%
11	3.698	744	749	753	rVB3	247	212	0.02%	0.003%
12	3.878	800	805	808	rBV2	271	313	0.03%	0.004%
13	3.994	837	841	843	rBV	300	257	0.03%	0.004%
14	4.036	850	854	855	rBV2	259	193	0.02%	0.003%
15	4.084	863	869	873	rBV2	199	247	0.03%	0.004%
16	4.206	901	907	909	rBV	261	229	0.02%	0.003%
17	4.264	921	925	928	rBV	255	226	0.02%	0.003%
18	4.338	943	948	952	rVV2	192	226	0.02%	0.003%
19	4.557	1012	1016	1020	rBV2	215	247	0.03%	0.004%
20	4.608	1021	1032	1059	rBV	58608	151023	15.76%	2.147%
21	4.936	1130	1134	1139	rBV2	270	341	0.04%	0.005%
22	5.052	1154	1170	1195	rBV	165016	364284	38.02%	5.179%
23	5.193	1212	1214	1217	rVB2	323	212	0.02%	0.003%
24	5.254	1229	1233	1239	rBV3	289	350	0.04%	0.005%
25	5.322	1241	1254	1273	rVB2	3403	7751	0.81%	0.110%
26	5.457	1293	1296	1302	rBV2	268	257	0.03%	0.004%
27	5.714	1356	1376	1407	rBV2	357092	958063	100.00%	13.622%
28	5.959	1446	1452	1455	rBV2	269	268	0.03%	0.004%
29	5.975	1455	1457	1461	rVB2	377	206	0.02%	0.003%
30	6.000	1461	1465	1467	rBV	334	310	0.03%	0.004%
31	6.103	1493	1497	1503	rBV3	218	253	0.03%	0.004%
32	6.238	1526	1539	1562	rBV	262827	508080	53.03%	7.224%
33	6.489	1613	1617	1620	rBV2	294	228	0.02%	0.003%
34	6.525	1623	1628	1631	rBV3	1091	1378	0.14%	0.020%
35	6.592	1643	1649	1650	rBV	355	344	0.04%	0.005%
36	6.682	1662	1677	1696	rBV	214693	423713	44.23%	6.024%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021924\
 Data File : VU057878.D
 Acq On : 19 Feb 2024 11:36
 Operator : MD/SY
 Sample : VU0219WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK040

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

37	6.779	1705	1707	1709	rVB2	543	209	0.02%	0.003%
38	6.807	1709	1716	1721	rBV3	803	820	0.09%	0.012%
39	7.029	1780	1785	1788	rBV2	305	383	0.04%	0.005%
40	7.097	1803	1806	1813	rVV2	237	217	0.02%	0.003%
41	7.161	1822	1826	1827	rBV2	311	212	0.02%	0.003%
42	7.557	1937	1949	1972	rBV	120189	217153	22.67%	3.087%
43	7.672	1979	1985	1998	rVB4	3137	5381	0.56%	0.077%
44	7.785	2016	2020	2022	rBV2	572	468	0.05%	0.007%
45	7.804	2024	2026	2031	rVB3	336	250	0.03%	0.004%
46	7.891	2040	2053	2077	rBV	425859	756136	78.92%	10.751%
47	8.094	2113	2116	2122	rVB3	337	296	0.03%	0.004%
48	8.123	2123	2125	2130	rVB3	329	242	0.03%	0.003%
49	8.174	2130	2141	2163	rBV	82300	143724	15.00%	2.043%
50	8.328	2183	2189	2194	rVB2	141	187	0.02%	0.003%
51	8.367	2197	2201	2204	rBV2	251	206	0.02%	0.003%
52	8.405	2210	2213	2218	rVB2	313	313	0.03%	0.004%
53	8.463	2222	2231	2236	rBV3	1351	1945	0.20%	0.028%
54	8.512	2243	2246	2250	rBV2	258	272	0.03%	0.004%
55	8.627	2271	2282	2324	rBV2	195549	400994	41.85%	5.701%
56	8.897	2363	2366	2368	rBV3	265	187	0.02%	0.003%
57	8.933	2373	2377	2379	rBV2	242	188	0.02%	0.003%
58	9.338	2495	2503	2507	rBV2	373	479	0.05%	0.007%
59	9.412	2513	2526	2550	rBV	373595	634287	66.21%	9.018%
60	9.569	2569	2575	2580	rBV2	579	651	0.07%	0.009%
61	9.698	2606	2615	2623	rBV3	1049	1737	0.18%	0.025%
62	10.103	2734	2741	2744	rBV4	778	1067	0.11%	0.015%
63	10.193	2766	2769	2774	rVB2	325	317	0.03%	0.005%
64	10.470	2850	2855	2856	rBV2	257	208	0.02%	0.003%
65	10.483	2856	2859	2862	rVV2	365	248	0.03%	0.004%
66	10.563	2879	2884	2888	rBV	336	310	0.03%	0.004%
67	10.637	2901	2907	2916	rVB5	1466	2116	0.22%	0.030%
68	10.672	2916	2918	2923	rVB3	319	229	0.02%	0.003%
69	10.749	2929	2942	2960	rBV	256173	423738	44.23%	6.025%
70	10.881	2974	2983	2994	rBV4	1786	3023	0.32%	0.043%
71	11.090	3043	3048	3049	rBV2	645	525	0.05%	0.007%
72	11.290	3105	3110	3114	rBV	285	340	0.04%	0.005%
73	11.331	3118	3123	3133	rVB2	333	549	0.06%	0.008%
74	11.383	3133	3139	3142	rBV2	410	506	0.05%	0.007%
75	11.470	3160	3166	3180	rVB4	1233	1790	0.19%	0.025%
76	11.563	3190	3195	3198	rBV2	317	274	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021924\
 Data File : VU057878.D
 Acq On : 19 Feb 2024 11:36
 Operator : MD/SY
 Sample : VU0219WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK040

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

77	11.746	3244	3252	3258	rBV5	2251	2908	0.30%	0.041%
78	11.807	3258	3271	3302	rBV	415361	682086	71.19%	9.698%
79	12.007	3329	3333	3338	rVB2	307	218	0.02%	0.003%
80	12.068	3347	3352	3357	rBV2	245	366	0.04%	0.005%
81	12.187	3376	3389	3409	rBV	380689	638535	66.65%	9.079%
82	12.354	3437	3441	3445	rVV2	350	314	0.03%	0.004%
83	12.576	3506	3510	3515	rBV	250	322	0.03%	0.005%
84	12.704	3547	3550	3556	rBV	302	341	0.04%	0.005%
85	12.765	3561	3569	3578	rVB2	4804	6972	0.73%	0.099%
86	13.003	3641	3643	3645	rVB2	398	181	0.02%	0.003%
87	13.039	3648	3654	3661	rBV2	264	374	0.04%	0.005%
88	13.074	3661	3665	3667	rBV2	248	206	0.02%	0.003%
89	13.225	3706	3712	3714	rBV3	2090	2258	0.24%	0.032%
90	13.505	3793	3799	3800	rBV2	330	281	0.03%	0.004%
91	13.595	3825	3827	3830	rBV	261	195	0.02%	0.003%
92	13.756	3873	3877	3880	rBV2	312	318	0.03%	0.005%
93	13.846	3897	3905	3916	rBV5	5964	9699	1.01%	0.138%
94	14.093	3972	3982	3999	rBV2	8339	16809	1.75%	0.239%
95	14.331	4046	4056	4069	rBV4	7486	12462	1.30%	0.177%
96	14.556	4122	4126	4127	rBV2	643	411	0.04%	0.006%
97	15.106	4292	4297	4300	rBV2	320	348	0.04%	0.005%
98	15.122	4300	4302	4306	rBV	312	224	0.02%	0.003%
99	15.396	4384	4387	4390	rBV2	400	332	0.03%	0.005%
100	15.907	4544	4546	4549	rBV2	522	315	0.03%	0.004%




Sum of corrected areas: 7033302

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021924\
Data File : VU057878.D
Acq On : 19 Feb 2024 11:36
Operator : MD/SY
Sample : VU0219WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK040

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

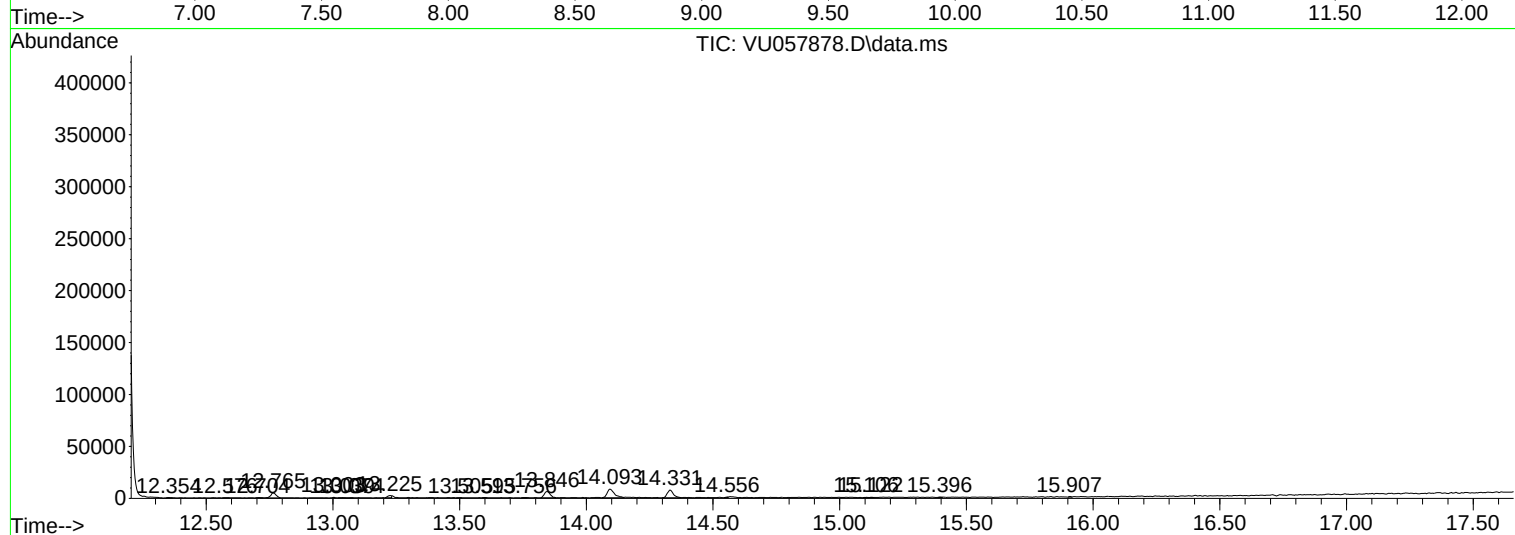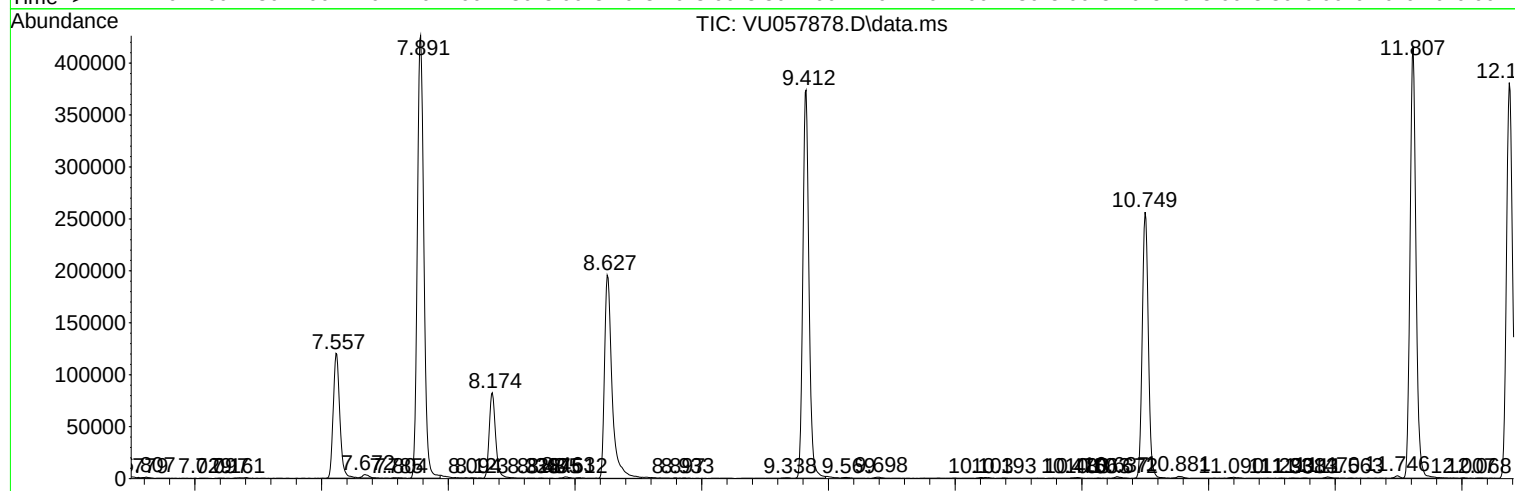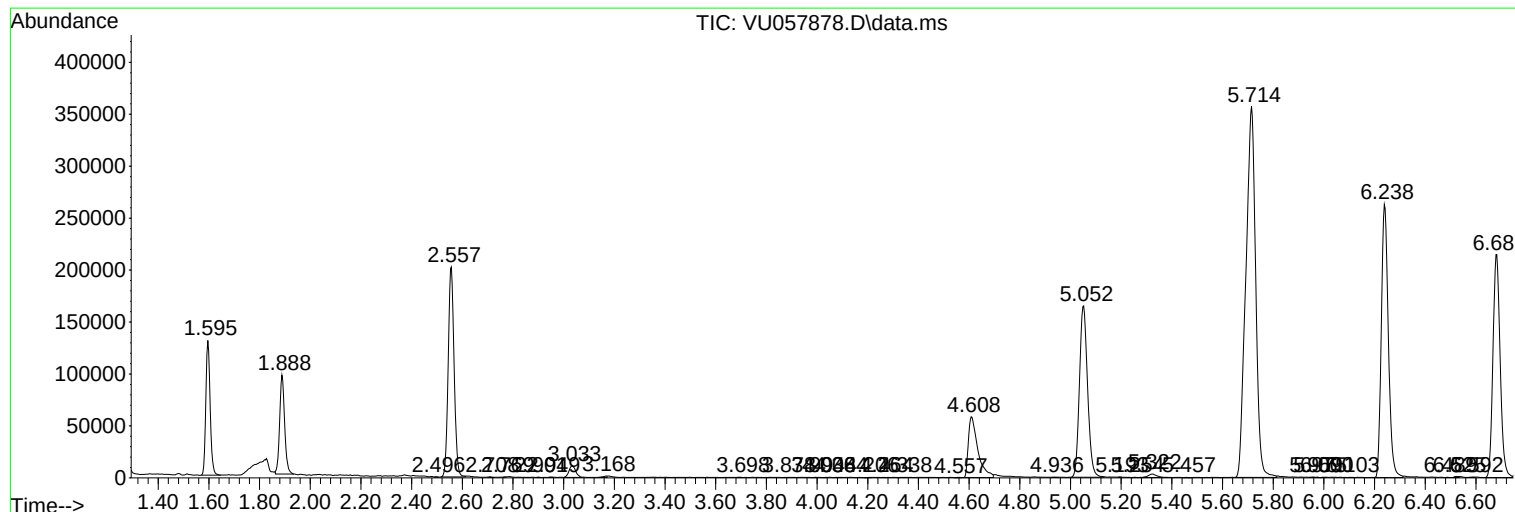

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021924\
Data File : VU057878.D
Acq On : 19 Feb 2024 11:36
Operator : MD/SY
Sample : VU0219WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK040

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021924\
Data File : VU057878.D
Acq On : 19 Feb 2024 11:36
Operator : MD/SY
Sample : VU0219WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK040

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------