

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021924\
 Data File : VU057879.D
 Acq On : 19 Feb 2024 12:04
 Operator : MD/SY
 Sample : P1513-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0U20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

Signal : TIC: VU057879.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	109	rVB	125318	147454	16.36%	2.105%
2	1.895	180	188	206	rVB	91219	128232	14.23%	1.830%
3	2.557	381	394	406	rBV	191785	313167	34.76%	4.470%
4	2.875	490	493	496	rBV	327	245	0.03%	0.003%
5	3.033	534	542	552	rBV4	2795	4541	0.50%	0.065%
6	3.177	575	587	600	rVB	2944	6153	0.68%	0.088%
7	3.319	617	631	637	rBV3	614	1482	0.16%	0.021%
8	3.435	664	667	672	rVB2	247	260	0.03%	0.004%
9	3.583	710	713	715	rBV2	263	189	0.02%	0.003%
10	3.859	791	799	803	rVB3	380	567	0.06%	0.008%
11	3.885	803	807	812	rBV2	250	268	0.03%	0.004%
12	4.033	849	853	859	rVB2	229	282	0.03%	0.004%
13	4.065	859	863	865	rBV2	287	230	0.03%	0.003%
14	4.113	871	878	882	rBV2	126	192	0.02%	0.003%
15	4.171	890	896	901	rBV2	270	325	0.04%	0.005%
16	4.206	903	907	909	rBV2	255	207	0.02%	0.003%
17	4.441	977	980	983	rBV	188	186	0.02%	0.003%
18	4.608	1021	1032	1061	rBV	53519	143460	15.92%	2.048%
19	5.052	1153	1170	1192	rBV	154519	343043	38.07%	4.896%
20	5.184	1209	1211	1215	rVB3	284	191	0.02%	0.003%
21	5.319	1242	1253	1254	rBV2	2121	2396	0.27%	0.034%
22	5.512	1309	1313	1318	rVB	223	234	0.03%	0.003%
23	5.714	1355	1376	1413	rBV2	333361	901059	100.00%	12.861%
24	6.065	1483	1485	1488	rVB2	364	193	0.02%	0.003%
25	6.193	1522	1525	1527	rBV	256	202	0.02%	0.003%
26	6.242	1527	1540	1561	rBV	282745	551962	61.26%	7.878%
27	6.534	1625	1631	1639	rVB6	824	1136	0.13%	0.016%
28	6.579	1639	1645	1647	rBV3	479	477	0.05%	0.007%
29	6.682	1663	1677	1704	rBV	203124	401425	44.55%	5.730%
30	6.962	1759	1764	1767	rBV3	974	1104	0.12%	0.016%
31	7.013	1776	1780	1786	rBV2	273	231	0.03%	0.003%
32	7.052	1789	1792	1795	rBV	217	221	0.02%	0.003%
33	7.174	1823	1830	1831	rBV2	389	345	0.04%	0.005%
34	7.193	1832	1836	1839	rBV3	568	431	0.05%	0.006%
35	7.447	1912	1915	1919	rBV	224	243	0.03%	0.003%
36	7.512	1931	1935	1938	rBV	249	212	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021924\
 Data File : VU057879.D
 Acq On : 19 Feb 2024 12:04
 Operator : MD/SY
 Sample : P1513-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0U20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

37	7.560	1938	1950	1973	rBV	115037	207512	23.03%	2.962%
38	7.676	1979	1986	2002	rVB4	2496	4069	0.45%	0.058%
39	7.891	2040	2053	2071	rBV	413142	717955	79.68%	10.248%
40	8.052	2099	2103	2105	rBV2	291	251	0.03%	0.004%
41	8.174	2129	2141	2163	rBV	78337	136143	15.11%	1.943%
42	8.396	2208	2210	2217	rVB	279	241	0.03%	0.003%
43	8.463	2222	2231	2241	rVV4	2008	3130	0.35%	0.045%
44	8.586	2264	2269	2271	rBV	192	194	0.02%	0.003%
45	8.627	2271	2282	2318	rBV	190161	375036	41.62%	5.353%
46	8.791	2328	2333	2344	rVB7	1772	2950	0.33%	0.042%
47	8.872	2356	2358	2361	rVB2	331	205	0.02%	0.003%
48	9.007	2396	2400	2403	rBV	207	211	0.02%	0.003%
49	9.335	2497	2502	2505	rBV2	403	391	0.04%	0.006%
50	9.412	2512	2526	2555	rBV	411611	707696	78.54%	10.101%
51	9.566	2570	2574	2582	rVB4	1005	1062	0.12%	0.015%
52	9.695	2605	2614	2627	rVB3	3748	6519	0.72%	0.093%
53	10.100	2732	2740	2750	rBV3	2377	3954	0.44%	0.056%
54	10.164	2756	2760	2765	rBV2	257	225	0.02%	0.003%
55	10.254	2782	2788	2799	rBV4	696	1337	0.15%	0.019%
56	10.354	2813	2819	2821	rVV2	245	242	0.03%	0.003%
57	10.479	2851	2858	2868	rVB3	2623	3942	0.44%	0.056%
58	10.569	2882	2886	2889	rBV2	269	195	0.02%	0.003%
59	10.624	2899	2903	2905	rBV2	232	187	0.02%	0.003%
60	10.749	2930	2942	2962	rBV	242109	395670	43.91%	5.647%
61	10.888	2976	2985	2991	rBV4	2555	4378	0.49%	0.062%
62	10.923	2991	2996	3004	rVB3	1051	1414	0.16%	0.020%
63	10.994	3014	3018	3019	rBV	270	206	0.02%	0.003%
64	11.097	3042	3050	3052	rBV2	775	941	0.10%	0.013%
65	11.187	3073	3078	3081	rBV2	247	284	0.03%	0.004%
66	11.235	3090	3093	3095	rBV	269	189	0.02%	0.003%
67	11.293	3106	3111	3113	rBV2	315	264	0.03%	0.004%
68	11.466	3158	3165	3174	rBV3	2028	3045	0.34%	0.043%
69	11.521	3179	3182	3185	rVB3	338	241	0.03%	0.003%
70	11.608	3204	3209	3212	rBV4	633	573	0.06%	0.008%
71	11.701	3235	3238	3240	rBV	304	248	0.03%	0.004%
72	11.746	3245	3252	3257	rBV4	1393	1616	0.18%	0.023%
73	11.807	3259	3271	3293	rBV	478937	778426	86.39%	11.111%
74	12.003	3328	3332	3335	rBV2	383	296	0.03%	0.004%
75	12.090	3349	3359	3366	rBV4	3687	5736	0.64%	0.082%
76	12.187	3376	3389	3417	rBV	376021	625741	69.45%	8.931%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021924\
 Data File : VU057879.D
 Acq On : 19 Feb 2024 12:04
 Operator : MD/SY
 Sample : P1513-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0U20

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
 Title : VOC Analysis

77	12.296	3418	3423	3433	rVB3	2037	3000	0.33%	0.043%
78	12.573	3505	3509	3511	rBV	529	400	0.04%	0.006%
79	12.614	3518	3522	3527	rBV2	339	376	0.04%	0.005%
80	12.682	3536	3543	3552	rBV5	1289	1920	0.21%	0.027%
81	12.765	3559	3569	3578	rBV2	5284	7898	0.88%	0.113%
82	12.859	3592	3598	3600	rBV2	703	678	0.08%	0.010%
83	12.942	3620	3624	3628	rBV2	484	533	0.06%	0.008%
84	12.974	3628	3634	3643	rVB5	1287	2356	0.26%	0.034%
85	13.032	3649	3652	3657	rVB2	399	286	0.03%	0.004%
86	13.110	3672	3676	3679	rBV2	426	364	0.04%	0.005%
87	13.222	3705	3711	3716	rBV4	1229	1716	0.19%	0.024%
88	13.325	3740	3743	3748	rVB2	427	281	0.03%	0.004%
89	13.454	3776	3783	3790	rVB5	1760	2571	0.29%	0.037%
90	13.560	3814	3816	3820	rVB2	487	239	0.03%	0.003%
91	13.765	3876	3880	3881	rBV2	305	223	0.02%	0.003%
92	13.846	3897	3905	3911	rBV5	3284	4744	0.53%	0.068%
93	13.894	3918	3920	3922	rBV3	574	319	0.04%	0.005%
94	14.097	3973	3983	4004	rVV2	6658	14159	1.57%	0.202%
95	14.190	4004	4012	4024	rVB6	2924	4265	0.47%	0.061%
96	14.283	4034	4041	4048	rVB4	3685	5002	0.56%	0.071%
97	14.331	4048	4056	4068	rBV5	3961	6054	0.67%	0.086%
98	14.457	4089	4095	4098	rBB3	395	390	0.04%	0.006%
99	14.569	4122	4130	4140	rBV2	1097	1944	0.22%	0.028%
100	14.807	4201	4204	4211	rVB3	864	955	0.11%	0.014%




Sum of corrected areas: 7006133

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021924\
Data File : VU057879.D
Acq On : 19 Feb 2024 12:04
Operator : MD/SY
Sample : P1513-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0U20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

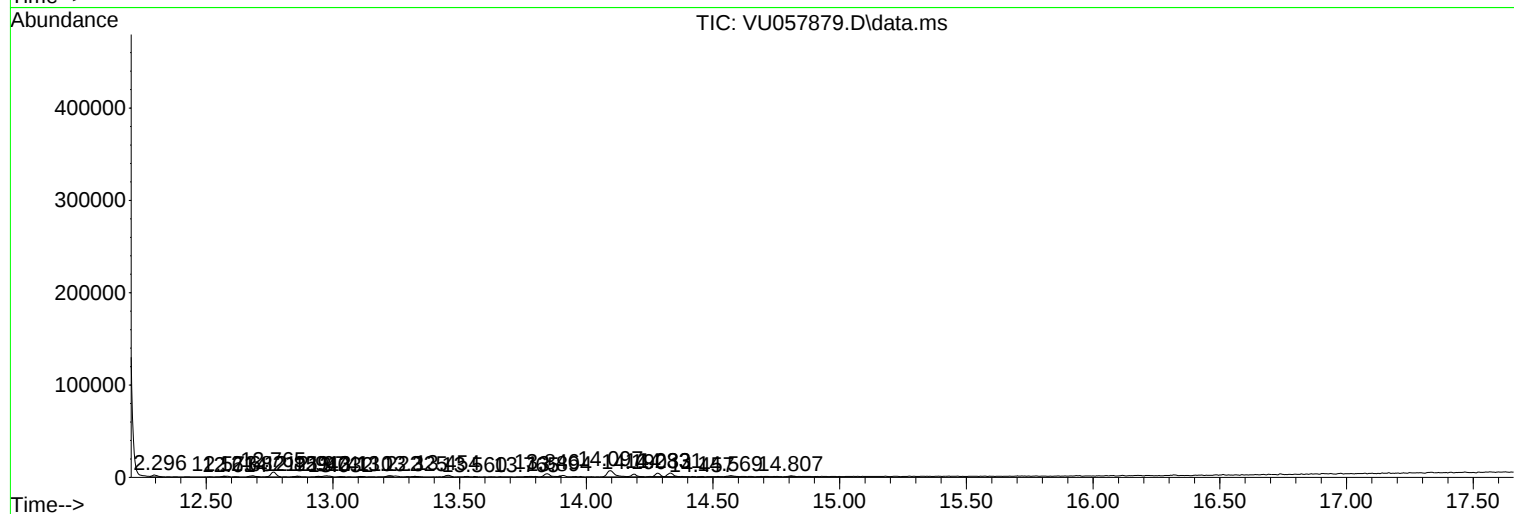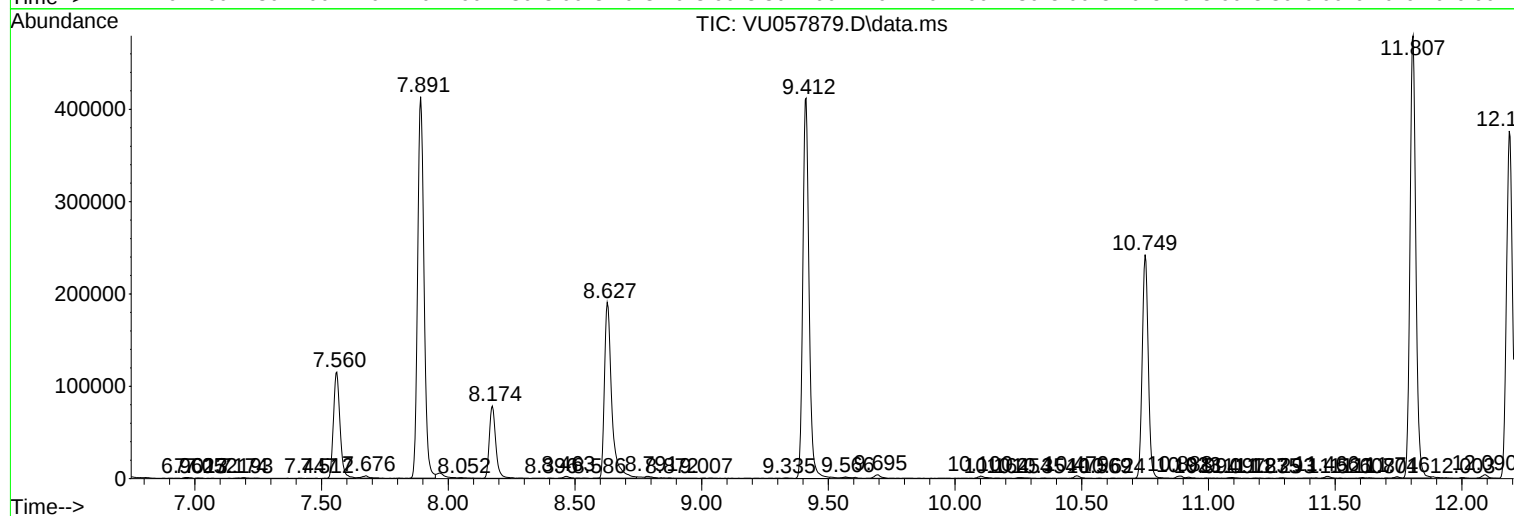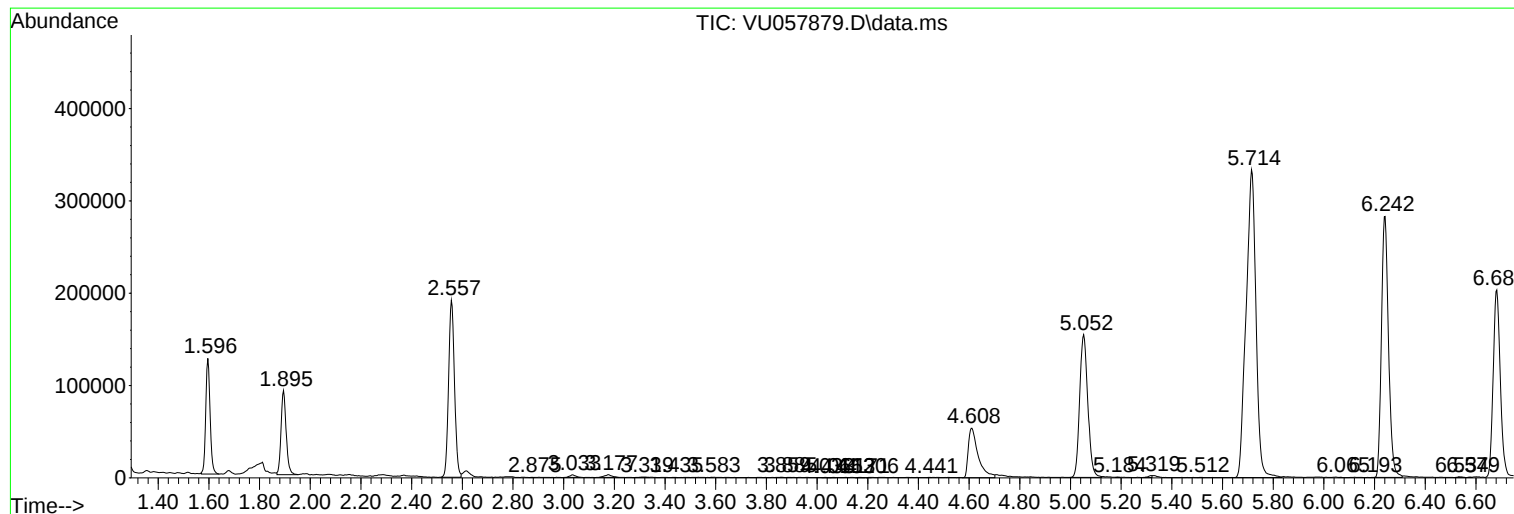

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021924\
Data File : VU057879.D
Acq On : 19 Feb 2024 12:04
Operator : MD/SY
Sample : P1513-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0U20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021924\
Data File : VU057879.D
Acq On : 19 Feb 2024 12:04
Operator : MD/SY
Sample : P1513-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0U20

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM020724WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------