


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021924\
Data File : VU057876.D
Acq On : 19 Feb 2024 08:19
Operator : MD/SY
Sample : BFB038
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB038

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Title : VOC Analysis
Last Update : Wed Feb 21 00:11:26 2024

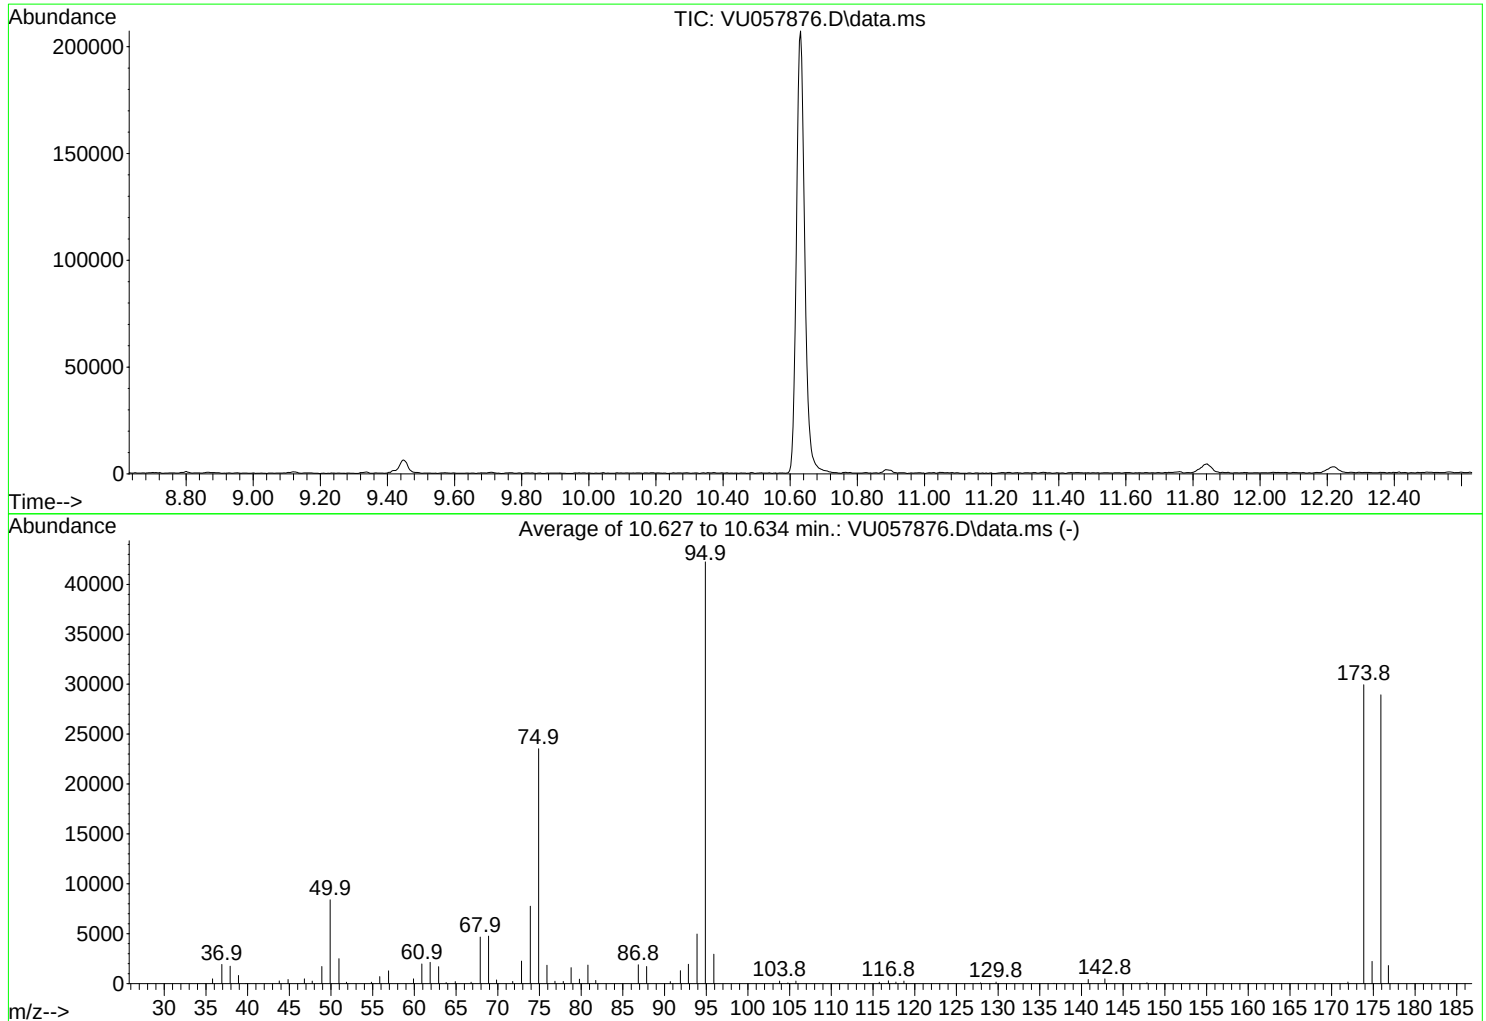

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.9	8405	PASS
75	95	30	80	55.7	23539	PASS
95	95	100	100	100.0	42256	PASS
96	95	5	9	7.0	2945	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	70.9	29939	PASS
175	174	5	9	7.4	2223	PASS
176	174	95	101	96.6	28931	PASS
177	176	5	9	6.2	1804	PASS

Scan 2892 (10.589 min): VU057876.D\data.ms
BFB038

m/z	Abundance
39.80	121.0
43.80	238.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038

m/z	Abundance
35.80	494.0
36.90	2007.0
37.90	1769.0
38.90	764.0
39.80	169.0
43.80	543.0
44.90	389.0
46.80	519.0
47.80	262.0
48.90	1722.0
49.90	8766.0
50.90	2644.0
51.90	151.0
54.80	138.0
55.90	856.0
56.90	1279.0
59.90	485.0
60.90	2031.0
61.90	2209.0
62.90	1824.0
63.80	134.0
64.90	161.0
66.80	150.0
67.90	4701.0
68.90	4829.0
69.90	409.0
71.90	263.0
72.90	2348.0
73.90	7886.0
74.90	23904.0
75.90	1934.0
76.80	263.0
77.90	234.0
78.80	1630.0
79.80	464.0
80.80	1771.0
81.70	313.0
86.80	1807.0
87.90	1636.0
90.70	227.0
91.90	1244.0
92.90	2031.0
93.90	4848.0
94.90	42288.0
95.90	3004.0
103.80	279.0
104.80	135.0
105.80	283.0
115.80	142.0
116.80	301.0
117.70	154.0
118.70	249.0
129.70	140.0
140.80	402.0
142.80	516.0
147.90	163.0
171.90	191.0
173.90	29856.0
174.90	2255.0
175.90	28312.0
176.80	1813.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038

m/z	Abundance
35.80	481.0
36.90	1937.0
37.90	1800.0
38.90	840.0
39.80	139.0
43.80	515.0
44.90	421.0
46.80	484.0
47.70	259.0
48.90	1756.0
49.90	8642.0
51.00	2537.0
51.80	157.0
54.80	145.0
55.80	710.0
56.90	1336.0
59.90	517.0
60.90	2019.0
61.90	2186.0
62.90	1727.0
63.80	117.0
64.90	227.0
66.80	146.0
67.90	4828.0
68.90	4883.0
69.80	373.0
71.80	208.0
72.90	2322.0
73.90	7943.0
74.90	24256.0
75.90	1869.0
76.80	246.0
77.90	253.0
78.80	1638.0
79.80	466.0
80.80	1930.0
81.80	311.0
86.90	1982.0
87.90	1738.0
90.70	219.0
91.90	1336.0
92.90	1975.0
93.90	5116.0
94.90	43512.0
95.90	3012.0
103.80	266.0
104.80	127.0
105.80	246.0
115.80	152.0
116.80	292.0
117.70	159.0
118.70	274.0
127.90	109.0
129.80	164.0
140.80	412.0
142.80	496.0
147.80	120.0
171.90	177.0
173.90	30664.0
174.90	2298.0
175.90	29992.0
176.80	1846.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038

m/z	Abundance
35.80	476.0
36.90	1816.0
37.90	1693.0
38.90	866.0
39.80	116.0
43.90	498.0
44.80	434.0
46.80	456.0
47.70	229.0
48.90	1665.0
49.90	7806.0
51.00	2330.0
51.80	111.0
54.90	152.0
55.80	545.0
56.90	1251.0
59.90	460.0
60.90	1867.0
61.90	2016.0
62.90	1539.0
63.80	107.0
64.90	252.0
66.80	133.0
67.90	4463.0
68.90	4590.0
69.90	341.0
71.70	182.0
72.80	2099.0
73.90	7462.0
74.90	22456.0
75.90	1746.0
76.90	225.0
77.80	203.0
78.80	1566.0
79.80	421.0
80.80	1880.0
81.80	317.0
86.90	1909.0
87.80	1768.0
90.70	194.0
91.90	1328.0
92.80	1823.0
93.90	4961.0
94.90	40968.0
95.90	2820.0
103.80	228.0
105.70	232.0
115.70	142.0
116.90	279.0
117.80	148.0
118.70	269.0
127.90	123.0
129.80	158.0
136.70	106.0
140.80	417.0
142.80	452.0
172.00	140.0
173.80	29296.0
174.80	2117.0
175.90	28488.0
176.80	1752.0

Instrument :
MSVOA_U
ClientSampleId :
BFB038