


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU021924\
Data File : VU057881.D
Acq On : 19 Feb 2024 15:02
Operator : MD/SY
Sample : BFB039
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB039

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Title : VOC Analysis
Last Update : Wed Feb 21 00:11:26 2024

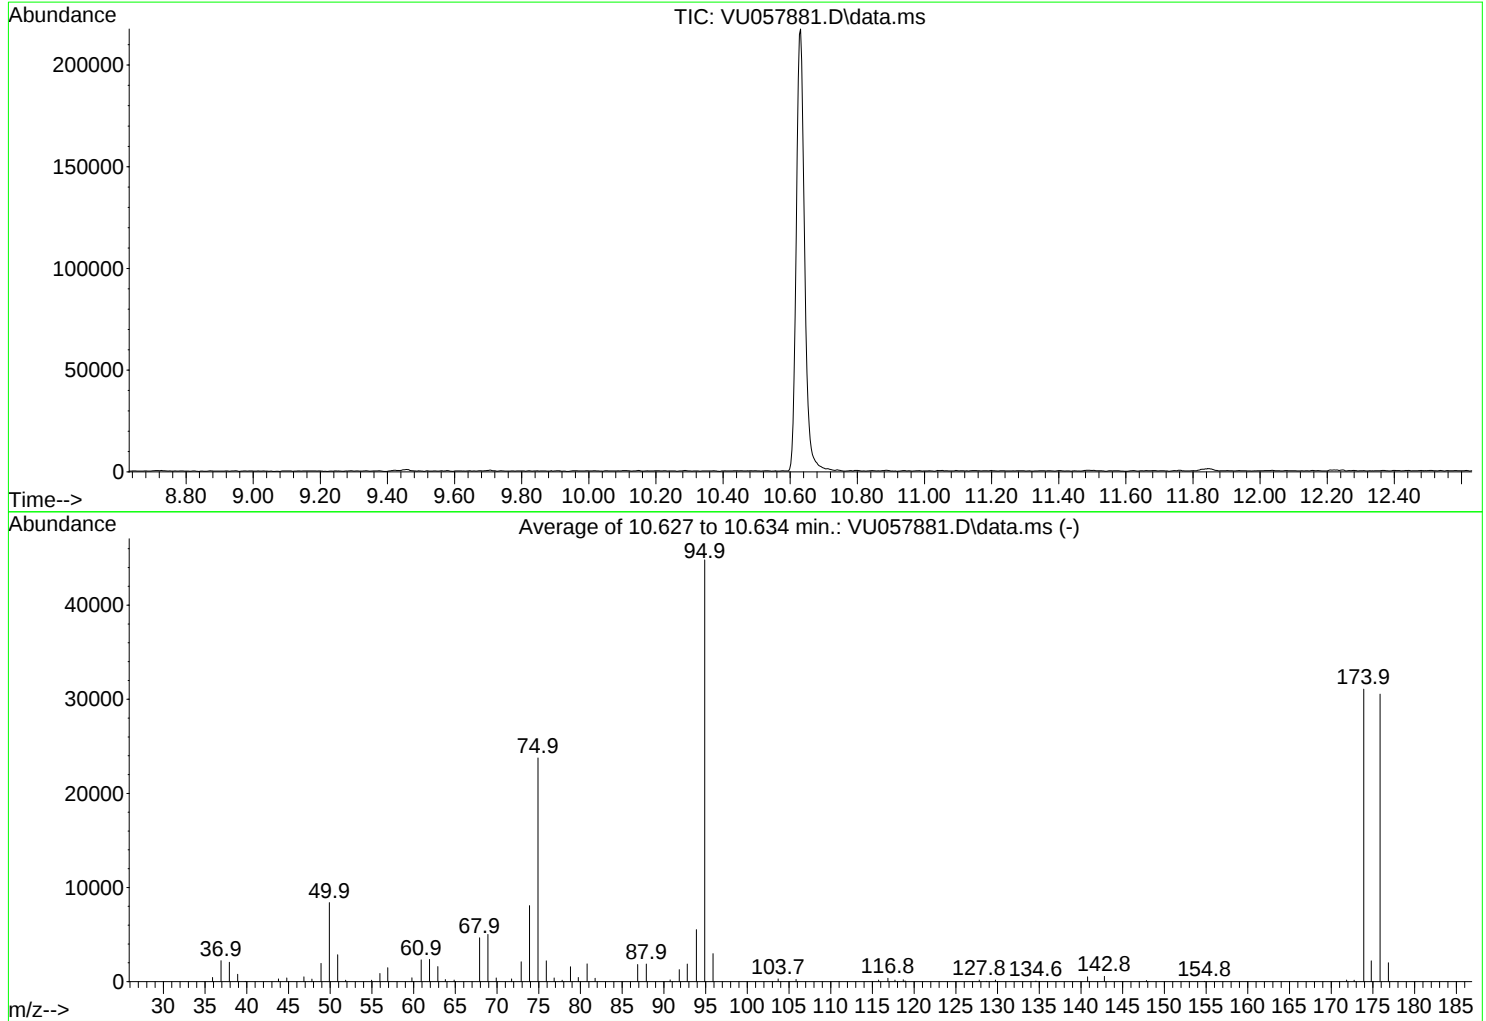

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2893

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.7	8401	PASS
75	95	30	80	53.0	23773	PASS
95	95	100	100	100.0	44813	PASS
96	95	5	9	6.6	2980	PASS
173	174	0.00	2	0.5	146	PASS
174	95	50	120	69.3	31077	PASS
175	174	5	9	7.1	2218	PASS
176	174	95	101	98.3	30549	PASS
177	176	5	9	6.6	2005	PASS

m/z	Abundance
39.80	156.0
43.80	347.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039

m/z	Abundance
35.90	440.0
36.90	2315.0
37.90	2172.0
38.90	817.0
39.80	190.0
43.90	636.0
44.80	391.0
46.80	563.0
47.80	302.0
48.90	1984.0
49.90	8410.0
50.90	2766.0
51.90	177.0
54.90	126.0
56.00	875.0
56.90	1518.0
59.80	381.0
60.90	2311.0
61.90	2409.0
62.90	1718.0
63.80	243.0
64.90	198.0
67.90	4815.0
68.90	5004.0
69.90	418.0
71.70	281.0
72.90	2159.0
73.90	8198.0
74.90	24648.0
75.90	2213.0
76.90	398.0
77.80	156.0
78.80	1609.0
79.70	503.0
80.80	1895.0
81.70	417.0
86.90	1909.0
87.90	1826.0
90.80	216.0
91.80	1335.0
92.80	2033.0
93.90	5693.0
94.90	45672.0
95.90	3096.0
103.70	265.0
105.90	254.0
115.70	181.0
116.80	321.0
117.70	157.0
118.70	314.0
127.80	174.0
128.70	101.0
129.80	161.0
134.60	124.0
140.80	487.0
142.80	618.0
147.90	141.0
171.80	151.0
173.90	31176.0
174.80	2261.0
175.90	30544.0
176.80	2145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039

m/z	Abundance
35.90	463.0
36.90	2300.0
37.90	2135.0
38.90	821.0
39.80	197.0
43.80	671.0
44.80	416.0
46.80	531.0
47.80	275.0
48.90	1990.0
49.90	8640.0
50.90	2957.0
51.80	166.0
55.00	146.0
55.90	903.0
56.90	1542.0
59.80	410.0
60.90	2401.0
61.90	2471.0
62.90	1634.0
63.80	244.0
64.80	170.0
67.90	4770.0
68.90	5186.0
69.90	425.0
71.80	298.0
72.90	2198.0
73.90	8298.0
74.90	24536.0
75.90	2314.0
76.90	415.0
77.80	140.0
78.80	1615.0
79.80	443.0
80.80	1934.0
81.80	369.0
86.80	1855.0
87.90	1917.0
90.70	180.0
91.90	1321.0
92.80	1893.0
93.90	5682.0
94.90	46072.0
95.90	3045.0
103.70	305.0
105.90	231.0
115.70	178.0
116.90	363.0
117.70	169.0
118.70	296.0
127.80	189.0
129.70	186.0
134.60	106.0
140.80	519.0
142.80	586.0
147.90	133.0
171.90	168.0
172.80	220.0
173.90	31784.0
174.80	2270.0
175.80	31488.0
176.90	2084.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039

m/z	Abundance
35.90	415.0
36.90	2069.0
37.90	1870.0
38.90	717.0
39.80	209.0
43.80	599.0
44.80	346.0
46.90	448.0
47.80	248.0
48.90	1841.0
49.90	8152.0
50.90	2830.0
51.80	127.0
55.00	179.0
55.90	811.0
56.90	1397.0
59.80	441.0
60.90	2230.0
61.90	2198.0
62.90	1469.0
63.80	202.0
64.80	147.0
67.90	4365.0
68.90	4841.0
69.90	336.0
71.80	290.0
72.90	1988.0
73.90	7751.0
74.90	22136.0
75.90	2110.0
76.80	384.0
77.80	141.0
78.80	1540.0
79.80	388.0
80.80	1847.0
81.80	312.0
86.80	1686.0
87.90	1853.0
90.80	164.0
91.90	1162.0
92.80	1679.0
93.90	5203.0
94.90	42696.0
95.90	2799.0
103.70	276.0
105.80	233.0
115.80	176.0
116.80	367.0
117.70	185.0
118.90	259.0
127.80	170.0
129.70	182.0
140.80	515.0
142.80	508.0
147.80	100.0
154.80	104.0
171.90	174.0
172.70	217.0
173.90	30272.0
174.80	2124.0
175.80	29616.0
176.90	1786.0

Instrument :
MSVOA_U
ClientSampleId :
BFB039