
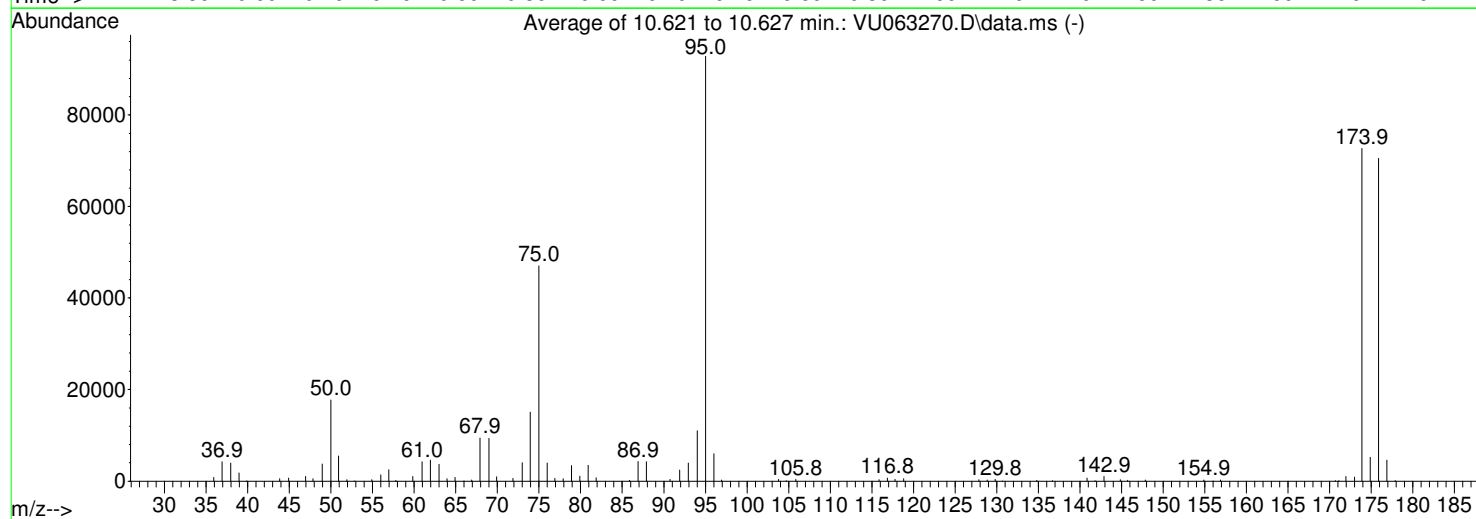


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022125\
Data File : VU063270.D
Acq On : 21 Feb 2025 11:56
Operator : MD/SY
Sample : BFB076
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB076

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR022125WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Mon Feb 24 11:41:21 2025

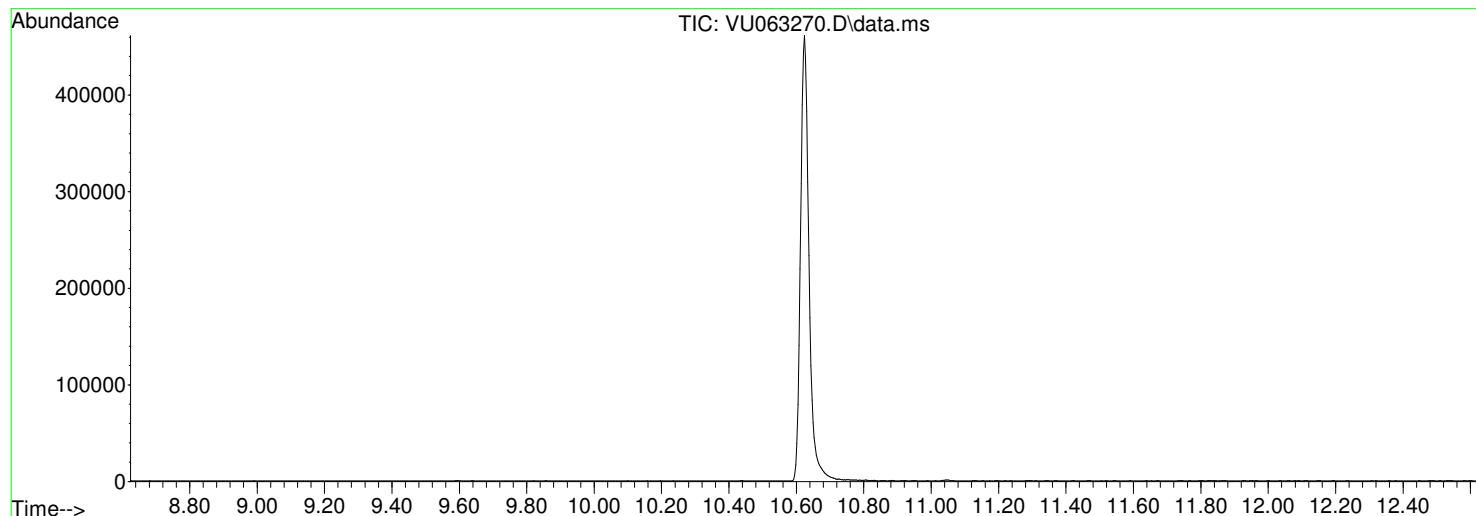

AutoFind: Scans 2902, 2903, 2904; Background Corrected with Scan 2889

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.1	17763	PASS
75	95	30	80	50.6	46989	PASS
95	95	100	100	100.0	92824	PASS
96	95	5	9	6.5	5990	PASS
173	174	0.00	2	1.2	897	PASS
174	95	50	120	78.3	72672	PASS
175	174	5	9	7.2	5221	PASS
176	174	95	101	97.0	70485	PASS
177	176	5	9	6.5	4589	PASS

m/z	Abundance
39.90	281.0
43.80	263.0

Instrument :
MSVOA_U
ClientSampleId :
BFB076

m/z	Abundance
35.90	839.0
36.90	4268.0
37.90	4104.0
38.90	1734.0
39.90	286.0
43.90	788.0
44.90	658.0
47.00	965.0
47.90	503.0
49.00	3778.0
50.00	17936.0
50.90	5663.0
51.90	290.0
52.80	114.0
54.90	338.0
56.00	1349.0
56.90	2408.0
57.80	152.0
59.90	998.0
61.00	4208.0
61.90	4656.0
63.00	3794.0
63.90	570.0
64.90	753.0
66.00	115.0
66.90	192.0
67.90	9830.0
69.00	9258.0
69.90	910.0
71.80	565.0
73.00	4148.0
74.00	15051.0
75.00	46224.0
76.00	4168.0
76.90	574.0
77.90	558.0
78.90	3458.0
79.90	1044.0
80.90	3644.0
81.80	740.0
85.90	153.0
86.90	4207.0
87.90	4148.0
90.70	358.0
91.90	2556.0
92.90	3892.0
94.00	11074.0
95.00	93312.0
96.00	6151.0
96.90	218.0
103.80	327.0
104.70	130.0
105.90	379.0
115.90	362.0
116.80	663.0
117.80	367.0
118.80	496.0
127.80	317.0
128.80	229.0
129.80	338.0
130.70	113.0
134.90	175.0
136.70	119.0
140.90	677.0
141.80	115.0
142.90	981.0
144.80	347.0
145.80	161.0
147.80	166.0
154.90	285.0
156.90	188.0
170.70	103.0
171.90	1077.0
173.00	968.0
173.90	70488.0
174.90	5078.0
175.90	68024.0
176.90	4663.0
177.90	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB076

m/z	Abundance
35.90	839.0
36.90	4354.0
37.90	4057.0
39.00	1869.0
39.90	283.0
43.90	769.0
44.90	690.0
47.00	1005.0
47.90	575.0
48.90	3877.0
50.00	18344.0
50.90	5620.0
51.90	309.0
54.90	306.0
56.00	1401.0
57.00	2550.0
57.80	160.0
59.80	1066.0
60.90	4422.0
62.00	4717.0
63.00	3792.0
64.00	521.0
64.90	800.0
66.90	285.0
67.90	9600.0
69.00	9608.0
69.90	969.0
71.80	574.0
73.00	4078.0
73.90	15383.0
75.00	48536.0
76.00	4052.0
76.90	602.0
77.90	541.0
78.90	3508.0
79.90	1085.0
80.90	3557.0
81.90	775.0
85.80	157.0
86.90	4477.0
87.90	4353.0
90.80	378.0
91.90	2425.0
93.00	4060.0
94.00	11354.0
95.00	95352.0
96.00	6123.0
96.90	250.0
103.80	348.0
104.70	133.0
105.90	375.0
115.80	362.0
116.80	673.0
117.80	399.0
118.80	541.0
127.90	314.0
128.80	226.0
129.80	360.0
130.70	106.0
134.80	170.0
136.70	114.0
140.80	690.0
141.80	116.0
142.90	1081.0
144.80	339.0
145.80	148.0
147.90	232.0
154.90	280.0
156.90	255.0
170.70	121.0
171.10	121.0
171.90	1038.0
173.00	917.0
173.90	74808.0
174.90	5333.0
175.90	72808.0
176.90	4728.0
177.90	134.0

Instrument :
MSVOA_U
ClientSampleId :
BFB076

m/z	Abundance
35.90	791.0
36.90	4079.0
38.00	3722.0
39.00	1819.0
39.80	306.0
43.90	715.0
44.90	676.0
46.90	1110.0
47.80	573.0
48.90	3572.0
50.00	17008.0
50.90	5125.0
51.90	262.0
54.90	250.0
56.00	1324.0
57.00	2596.0
57.80	141.0
59.80	995.0
60.90	4164.0
62.00	4461.0
63.00	3511.0
64.00	469.0
64.90	809.0
66.90	302.0
67.90	8694.0
69.00	9129.0
69.90	893.0
71.90	569.0
73.00	3865.0
73.90	14841.0
75.00	46208.0
76.00	3628.0
76.90	527.0
77.90	451.0
78.90	3183.0
79.90	1046.0
80.90	3236.0
81.90	732.0
85.80	156.0
86.90	4161.0
87.90	4143.0
90.80	336.0
91.90	2231.0
93.00	3930.0
94.00	10701.0
95.00	89808.0
96.00	5695.0
97.00	248.0
103.80	407.0
105.80	334.0
115.80	316.0
116.90	613.0
117.80	348.0
118.80	617.0
127.90	310.0
128.90	180.0
129.80	391.0
134.70	135.0
136.70	111.0
140.80	672.0
142.90	1080.0
144.90	291.0
145.70	123.0
147.80	256.0
154.90	241.0
156.00	100.0
156.90	244.0
170.70	137.0
171.10	118.0
172.00	967.0
173.00	807.0
173.90	72720.0
174.90	5251.0
175.90	70624.0
176.90	4376.0
177.90	110.0

Instrument :
MSVOA_U
ClientSampleId :
BFB076