

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
 Data File : VU057940.D
 Acq On : 23 Feb 2024 10:26
 Operator : MD/SY
 Sample : VU0223WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK044

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M

Title : VOC Analysis

Signal : TIC: VU057940.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.595	87	95	107	rBV	110600	124175	13.74%	1.749%
2	1.907	184	192	204	rVB	90686	116640	12.90%	1.643%
3	2.560	382	395	413	rBV	177824	293756	32.50%	4.138%
4	2.701	437	439	441	rVV3	294	184	0.02%	0.003%
5	2.782	458	464	475	rBV2	1601	2748	0.30%	0.039%
6	2.843	481	483	485	rBV2	271	180	0.02%	0.003%
7	3.029	535	541	542	rBV2	1154	904	0.10%	0.013%
8	3.081	555	557	563	rVB2	318	279	0.03%	0.004%
9	3.161	579	582	583	rBV	314	204	0.02%	0.003%
10	3.351	634	641	650	rVB2	1286	1750	0.19%	0.025%
11	3.457	671	674	680	rBV	196	189	0.02%	0.003%
12	3.782	771	775	779	rVB2	219	189	0.02%	0.003%
13	3.808	779	783	785	rBV	231	210	0.02%	0.003%
14	3.943	818	825	826	rBV	211	243	0.03%	0.003%
15	3.962	826	831	836	rBV2	171	238	0.03%	0.003%
16	4.007	838	845	850	rBV2	273	437	0.05%	0.006%
17	4.193	900	903	905	rBV2	188	150	0.02%	0.002%
18	4.316	937	941	947	rBV2	193	175	0.02%	0.002%
19	4.351	949	952	957	rVB	322	291	0.03%	0.004%
20	4.409	964	970	973	rBV	171	249	0.03%	0.004%
21	4.441	974	980	983	rBV2	164	219	0.02%	0.003%
22	4.508	996	1001	1004	rBV	176	199	0.02%	0.003%
23	4.608	1023	1032	1072	rBV	58593	163722	18.11%	2.306%
24	4.968	1137	1144	1147	rVB3	429	420	0.05%	0.006%
25	4.988	1147	1150	1155	rBV2	207	227	0.03%	0.003%
26	5.052	1155	1170	1196	rBV	159999	359469	39.76%	5.063%
27	5.367	1265	1268	1271	rBV2	268	182	0.02%	0.003%
28	5.534	1314	1320	1321	rBV	198	148	0.02%	0.002%
29	5.717	1357	1377	1404	rBV2	325767	903989	100.00%	12.733%
30	6.000	1462	1465	1468	rBV	396	253	0.03%	0.004%
31	6.039	1475	1477	1481	rVB2	319	197	0.02%	0.003%
32	6.119	1498	1502	1506	rBV2	294	226	0.03%	0.003%
33	6.174	1516	1519	1523	rVB2	212	168	0.02%	0.002%
34	6.242	1527	1540	1560	rBV	332637	652346	72.16%	9.188%
35	6.473	1609	1612	1616	rBV2	356	273	0.03%	0.004%
36	6.531	1621	1630	1640	rVB5	2145	3686	0.41%	0.052%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
 Data File : VU057940.D
 Acq On : 23 Feb 2024 10:26
 Operator : MD/SY
 Sample : VU0223WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK044

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

37	6.605	1650	1653	1656	rVB2	282	226	0.03%	0.003%
38	6.682	1664	1677	1700	rBV	206085	413416	45.73%	5.823%
39	6.840	1724	1726	1728	rBV	444	183	0.02%	0.003%
40	6.901	1741	1745	1750	rBV2	168	161	0.02%	0.002%
41	7.010	1776	1779	1784	rBV2	292	292	0.03%	0.004%
42	7.036	1784	1787	1790	rBV2	197	153	0.02%	0.002%
43	7.103	1806	1808	1814	rVB	370	342	0.04%	0.005%
44	7.261	1854	1857	1859	rBV	228	181	0.02%	0.003%
45	7.486	1923	1927	1929	rBV	248	196	0.02%	0.003%
46	7.560	1938	1950	1974	rBV	111479	208295	23.04%	2.934%
47	7.711	1992	1997	2001	rBV4	584	527	0.06%	0.007%
48	7.788	2018	2021	2022	rBV2	257	178	0.02%	0.003%
49	7.891	2039	2053	2090	rBV	402090	712430	78.81%	10.035%
50	8.174	2130	2141	2165	rBV	74832	136442	15.09%	1.922%
51	8.547	2252	2257	2263	rBV5	474	498	0.06%	0.007%
52	8.627	2270	2282	2317	rBV3	178373	397477	43.97%	5.599%
53	8.923	2369	2374	2376	rBV2	565	466	0.05%	0.007%
54	9.113	2427	2433	2436	rBV	171	198	0.02%	0.003%
55	9.209	2461	2463	2466	rBV	184	155	0.02%	0.002%
56	9.412	2512	2526	2564	rBV	469278	809704	89.57%	11.405%
57	9.566	2570	2574	2580	rVB3	892	970	0.11%	0.014%
58	9.682	2606	2610	2611	rBV2	298	187	0.02%	0.003%
59	9.698	2611	2615	2621	rVB	713	776	0.09%	0.011%
60	9.743	2626	2629	2631	rBV2	237	183	0.02%	0.003%
61	9.958	2692	2696	2697	rBV	226	154	0.02%	0.002%
62	10.110	2735	2743	2744	rBV3	711	752	0.08%	0.011%
63	10.119	2744	2746	2750	rVB2	500	416	0.05%	0.006%
64	10.164	2756	2760	2763	rBV2	212	206	0.02%	0.003%
65	10.306	2800	2804	2806	rBV	341	253	0.03%	0.004%
66	10.425	2838	2841	2846	rBV2	278	284	0.03%	0.004%
67	10.479	2855	2858	2863	rBV3	545	590	0.07%	0.008%
68	10.518	2867	2870	2876	rVB	194	166	0.02%	0.002%
69	10.643	2906	2909	2913	rBV	324	339	0.04%	0.005%
70	10.749	2929	2942	2963	rVV	247064	404677	44.77%	5.700%
71	10.952	3001	3005	3011	rBV2	313	315	0.03%	0.004%
72	11.000	3016	3020	3023	rBV	182	170	0.02%	0.002%
73	11.093	3042	3049	3056	rBV2	677	1027	0.11%	0.014%
74	11.145	3062	3065	3068	rBV	244	202	0.02%	0.003%
75	11.219	3084	3088	3094	rBV2	225	303	0.03%	0.004%
76	11.331	3119	3123	3126	rBV	205	225	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
 Data File : VU057940.D
 Acq On : 23 Feb 2024 10:26
 Operator : MD/SY
 Sample : VU0223WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK044

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

77	11.466	3160	3165	3179	rVB3	1338	2286	0.25%	0.032%
78	11.527	3179	3184	3191	rBV2	273	420	0.05%	0.006%
79	11.666	3223	3227	3228	rBV	208	171	0.02%	0.002%
80	11.746	3243	3252	3259	rBV	2346	3187	0.35%	0.045%
81	11.807	3259	3271	3292	rBV	455188	744864	82.40%	10.492%
82	12.113	3359	3366	3367	rBV2	263	288	0.03%	0.004%
83	12.187	3377	3389	3412	rBV	351168	586675	64.90%	8.263%
84	12.765	3566	3569	3570	rBV2	221	148	0.02%	0.002%
85	12.897	3608	3610	3616	rBV2	224	224	0.02%	0.003%
86	12.923	3616	3618	3623	rVB2	244	152	0.02%	0.002%
87	13.080	3665	3667	3672	rBV	298	271	0.03%	0.004%
88	13.228	3705	3713	3724	rVB4	2534	3970	0.44%	0.056%
89	13.379	3757	3760	3764	rBV2	178	196	0.02%	0.003%
90	13.425	3770	3774	3778	rBV2	332	290	0.03%	0.004%
91	13.630	3836	3838	3842	rVB	321	240	0.03%	0.003%
92	13.846	3897	3905	3920	rVB6	5034	8352	0.92%	0.118%
93	13.949	3934	3937	3938	rBV6	279	148	0.02%	0.002%
94	14.093	3972	3982	3997	rBV3	6288	13462	1.49%	0.190%
95	14.228	4021	4024	4027	rBV2	278	182	0.02%	0.003%
96	14.331	4047	4056	4067	rBV5	6338	10433	1.15%	0.147%
97	14.566	4126	4129	4131	rBV	235	177	0.02%	0.002%
98	14.682	4162	4165	4167	rBV3	347	241	0.03%	0.003%
99	14.727	4176	4179	4184	rBV3	367	450	0.05%	0.006%
100	15.601	4449	4451	4452	rBV	385	150	0.02%	0.002%




Sum of corrected areas: 7099607

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
Data File : VU057940.D
Acq On : 23 Feb 2024 10:26
Operator : MD/SY
Sample : VU0223WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK044

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

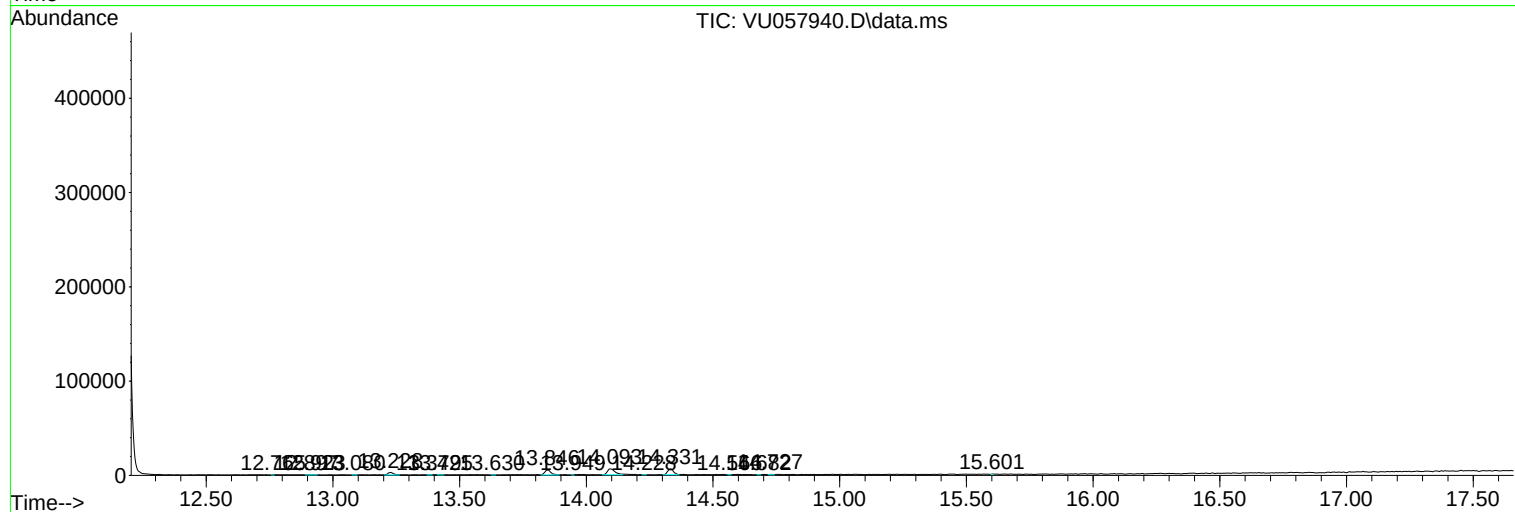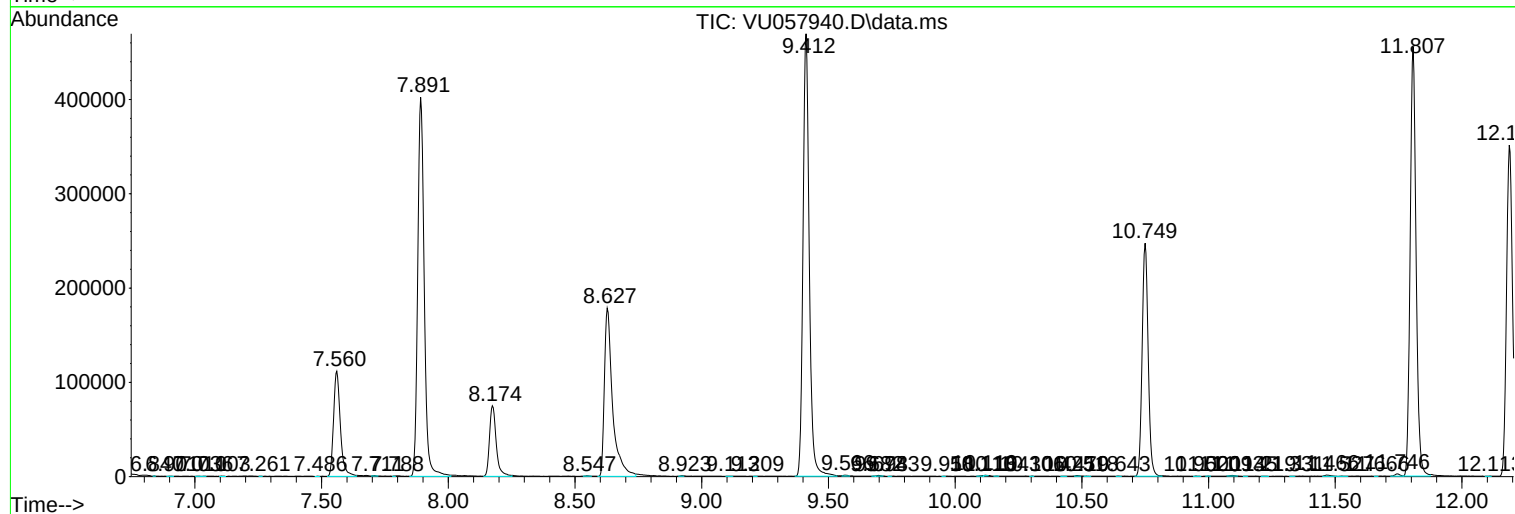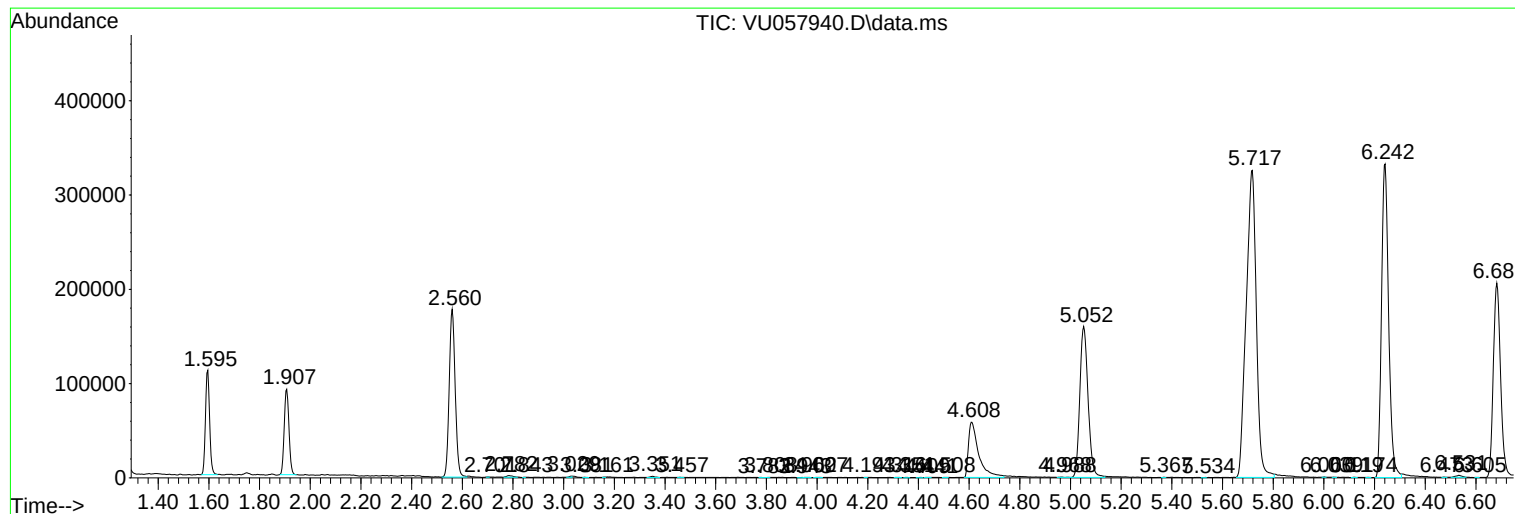

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
Data File : VU057940.D
Acq On : 23 Feb 2024 10:26
Operator : MD/SY
Sample : VU0223WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK044

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
Data File : VU057940.D
Acq On : 23 Feb 2024 10:26
Operator : MD/SY
Sample : VU0223WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK044

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------