

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
 Data File : VU057943.D
 Acq On : 23 Feb 2024 11:56
 Operator : MD/SY
 Sample : P1567-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JWAD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

Signal : TIC: VU057943.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	87	94	110	rVB	106485	122388	13.92%	1.760%
2	1.908	183	192	205	rVB	87583	113028	12.85%	1.625%
3	2.560	382	395	407	rBV	172276	284463	32.35%	4.091%
4	2.740	443	451	459	rBV	4396	7807	0.89%	0.112%
5	3.030	534	541	542	rBV3	1181	1055	0.12%	0.015%
6	3.145	574	577	578	rBV	326	213	0.02%	0.003%
7	3.174	578	586	596	rVB4	1395	2688	0.31%	0.039%
8	3.297	620	624	631	rVB	405	585	0.07%	0.008%
9	3.345	631	639	646	rBV4	795	1286	0.15%	0.018%
10	3.454	669	673	676	rVB	242	235	0.03%	0.003%
11	3.473	676	679	683	rBV	157	155	0.02%	0.002%
12	3.506	686	689	694	rBV2	192	175	0.02%	0.003%
13	3.814	780	785	787	rBV2	182	219	0.02%	0.003%
14	3.991	837	840	844	rVB2	238	197	0.02%	0.003%
15	4.039	850	855	863	rBV2	340	529	0.06%	0.008%
16	4.078	863	867	871	rBV2	220	275	0.03%	0.004%
17	4.361	952	955	959	rBV	246	238	0.03%	0.003%
18	4.525	1003	1006	1011	rBV	306	341	0.04%	0.005%
19	4.560	1011	1017	1021	rBV2	185	210	0.02%	0.003%
20	4.612	1021	1033	1066	rBV2	54593	150956	17.17%	2.171%
21	5.052	1154	1170	1193	rBV	155613	349641	39.76%	5.028%
22	5.290	1238	1244	1247	rBV3	208	254	0.03%	0.004%
23	5.345	1258	1261	1264	rBV2	262	219	0.02%	0.003%
24	5.460	1292	1297	1300	rVB2	255	269	0.03%	0.004%
25	5.718	1355	1377	1405	rBV2	317817	879317	100.00%	12.645%
26	5.952	1448	1450	1457	rVB3	233	192	0.02%	0.003%
27	6.033	1469	1475	1477	rBV2	417	378	0.04%	0.005%
28	6.116	1497	1501	1503	rBV	265	172	0.02%	0.002%
29	6.181	1518	1521	1527	rBV	199	270	0.03%	0.004%
30	6.242	1527	1540	1564	rBV	340760	665759	75.71%	9.574%
31	6.496	1616	1619	1623	rBV3	167	160	0.02%	0.002%
32	6.538	1623	1632	1644	rVB4	8762	16576	1.89%	0.238%
33	6.595	1647	1650	1655	rVB	281	214	0.02%	0.003%
34	6.682	1664	1677	1703	rBV	201376	402564	45.78%	5.789%
35	6.801	1711	1714	1720	rVB4	743	670	0.08%	0.010%
36	6.843	1725	1727	1735	rVB3	316	278	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
 Data File : VU057943.D
 Acq On : 23 Feb 2024 11:56
 Operator : MD/SY
 Sample : P1567-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JWAD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

37	7.017	1777	1781	1783	rVB2	243	179	0.02%	0.003%
38	7.103	1802	1808	1811	rBV2	178	174	0.02%	0.003%
39	7.177	1828	1831	1832	rBV	259	172	0.02%	0.002%
40	7.197	1832	1837	1840	rVV	337	381	0.04%	0.005%
41	7.412	1901	1904	1912	rVB2	239	235	0.03%	0.003%
42	7.480	1922	1925	1931	rVB2	207	203	0.02%	0.003%
43	7.560	1938	1950	1973	rBV	109360	200350	22.78%	2.881%
44	7.673	1982	1985	1990	rVB3	715	608	0.07%	0.009%
45	7.801	2020	2025	2028	rVB3	286	267	0.03%	0.004%
46	7.891	2036	2053	2071	rBV	380955	677798	77.08%	9.747%
47	8.174	2128	2141	2170	rBV	72022	131844	14.99%	1.896%
48	8.441	2219	2224	2227	rBV2	264	179	0.02%	0.003%
49	8.470	2227	2233	2237	rBV3	432	622	0.07%	0.009%
50	8.550	2253	2258	2263	rVB4	564	526	0.06%	0.008%
51	8.627	2271	2282	2314	rBV3	166069	377928	42.98%	5.435%
52	9.004	2395	2399	2401	rBV	256	202	0.02%	0.003%
53	9.158	2440	2447	2453	rBV2	324	552	0.06%	0.008%
54	9.219	2461	2466	2471	rBV2	277	350	0.04%	0.005%
55	9.280	2481	2485	2491	rBV2	214	245	0.03%	0.004%
56	9.325	2496	2499	2501	rBV2	234	183	0.02%	0.003%
57	9.412	2513	2526	2562	rBV	474246	811389	92.27%	11.669%
58	9.570	2571	2575	2581	rVB3	796	678	0.08%	0.010%
59	9.692	2607	2613	2615	rBV3	604	608	0.07%	0.009%
60	9.907	2677	2680	2686	rBV	187	165	0.02%	0.002%
61	10.029	2712	2718	2720	rBV	346	459	0.05%	0.007%
62	10.100	2735	2740	2743	rVV2	304	321	0.04%	0.005%
63	10.258	2786	2789	2791	rBV	210	171	0.02%	0.002%
64	10.341	2811	2815	2817	rBV2	285	242	0.03%	0.003%
65	10.412	2834	2837	2842	rVB2	261	231	0.03%	0.003%
66	10.438	2842	2845	2848	rBV	201	193	0.02%	0.003%
67	10.560	2879	2883	2885	rBV2	208	187	0.02%	0.003%
68	10.647	2907	2910	2914	rBV	275	260	0.03%	0.004%
69	10.705	2924	2928	2930	rBV2	364	330	0.04%	0.005%
70	10.750	2930	2942	2963	rVV	240258	393559	44.76%	5.660%
71	10.888	2976	2985	2989	rBV4	637	1035	0.12%	0.015%
72	10.971	3005	3011	3012	rBV	230	264	0.03%	0.004%
73	11.068	3032	3041	3046	rBV3	412	570	0.06%	0.008%
74	11.119	3052	3057	3059	rBV2	174	156	0.02%	0.002%
75	11.393	3137	3142	3145	rBV2	257	261	0.03%	0.004%
76	11.582	3196	3201	3205	rBV2	297	396	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
 Data File : VU057943.D
 Acq On : 23 Feb 2024 11:56
 Operator : MD/SY
 Sample : P1567-18
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 JWAD7

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

77	11.621	3210	3213	3215	rBV2	290	234	0.03%	0.003%
78	11.750	3246	3253	3257	rVB3	1056	963	0.11%	0.014%
79	11.807	3258	3271	3296	rBV	466856	762665	86.73%	10.968%
80	11.955	3315	3317	3320	rBV2	320	201	0.02%	0.003%
81	12.081	3346	3356	3359	rBV4	1979	3185	0.36%	0.046%
82	12.187	3377	3389	3416	rBV	341048	571941	65.04%	8.225%
83	12.357	3439	3442	3445	rVB	482	363	0.04%	0.005%
84	12.380	3445	3449	3452	rBV2	285	288	0.03%	0.004%
85	12.457	3469	3473	3474	rBV2	204	156	0.02%	0.002%
86	12.486	3478	3482	3484	rBV	315	222	0.03%	0.003%
87	12.868	3597	3601	3603	rBV	254	213	0.02%	0.003%
88	13.004	3639	3643	3644	rBV2	262	189	0.02%	0.003%
89	13.055	3653	3659	3662	rBV	289	319	0.04%	0.005%
90	13.222	3708	3711	3713	rBV2	543	361	0.04%	0.005%
91	13.473	3786	3789	3792	rBV2	264	212	0.02%	0.003%
92	13.746	3871	3874	3875	rBV	223	155	0.02%	0.002%
93	13.852	3901	3907	3914	rBV	1136	1143	0.13%	0.016%
94	14.077	3974	3977	3979	rBV	256	153	0.02%	0.002%
95	14.267	4032	4036	4039	rBV2	344	243	0.03%	0.003%
96	14.528	4110	4117	4121	rBV3	426	647	0.07%	0.009%
97	15.016	4266	4269	4270	rBV	310	185	0.02%	0.003%
98	15.216	4329	4331	4334	rBV	265	181	0.02%	0.003%
99	16.437	4709	4711	4715	rBV3	777	433	0.05%	0.006%
100	16.457	4715	4717	4720	rBV2	788	499	0.06%	0.007%




Sum of corrected areas: 6953600

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
Data File : VU057943.D
Acq On : 23 Feb 2024 11:56
Operator : MD/SY
Sample : P1567-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JWAD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

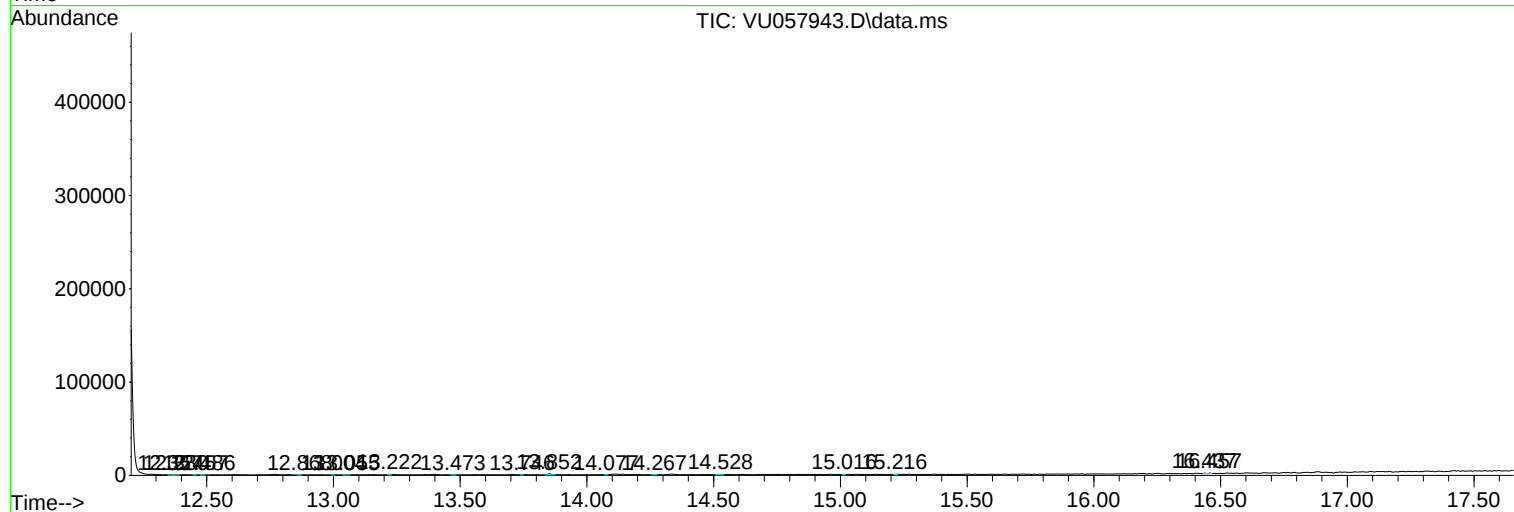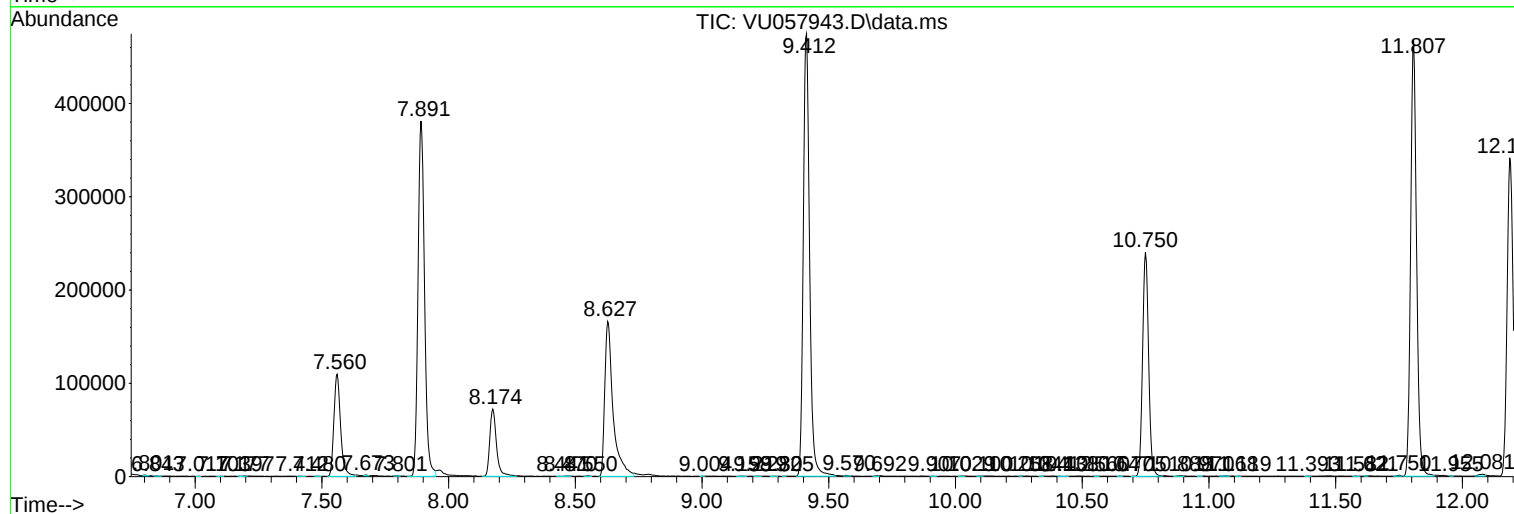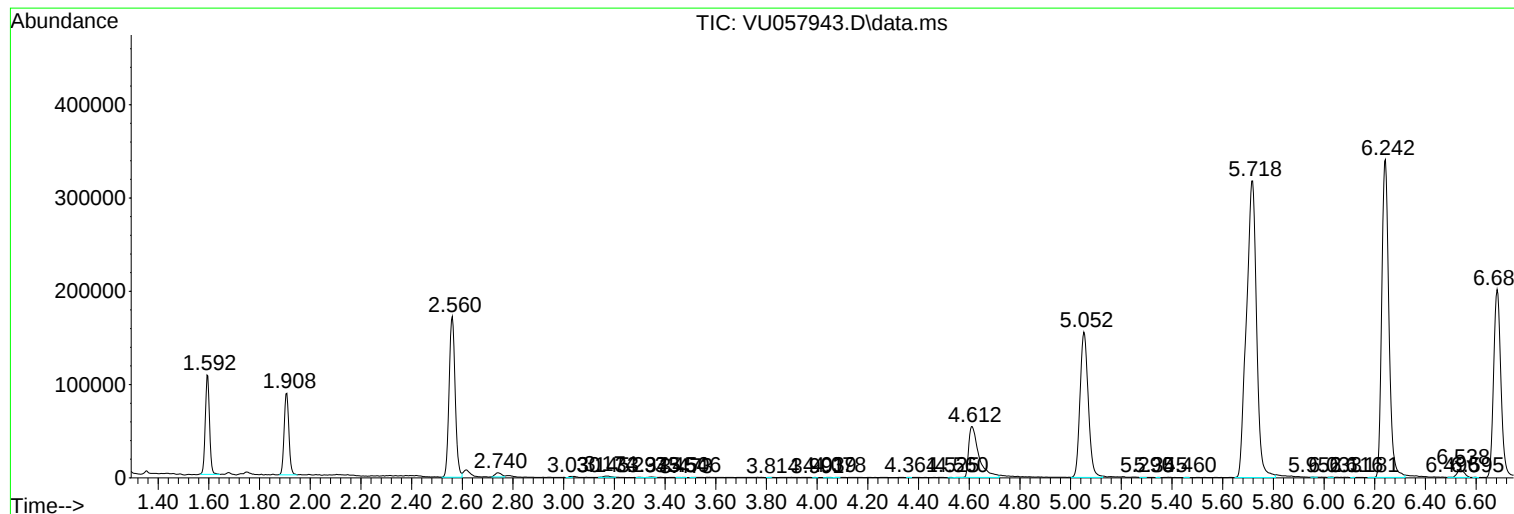

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
Data File : VU057943.D
Acq On : 23 Feb 2024 11:56
Operator : MD/SY
Sample : P1567-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JWAD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
Data File : VU057943.D
Acq On : 23 Feb 2024 11:56
Operator : MD/SY
Sample : P1567-18
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
JWAD7

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------