

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
 Data File : VU057944.D
 Acq On : 23 Feb 2024 12:55
 Operator : MD/SY
 Sample : P1567-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

Signal : TIC: VU057944.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.596	87	95	112	rVB	111196	126550	13.30%	1.714%
2	1.907	183	192	205	rVB	94544	121291	12.75%	1.642%
3	2.560	382	395	415	rBV	186538	305031	32.07%	4.131%
4	2.779	458	463	464	rBV2	334	278	0.03%	0.004%
5	2.853	483	486	490	rBV3	351	316	0.03%	0.004%
6	2.940	509	513	515	rBV2	253	212	0.02%	0.003%
7	2.978	521	525	526	rBV	307	239	0.03%	0.003%
8	3.036	536	543	552	rVB4	1812	3111	0.33%	0.042%
9	3.075	553	555	561	rVB2	269	181	0.02%	0.002%
10	3.104	561	564	568	rBV	296	241	0.03%	0.003%
11	3.126	568	571	575	rBV2	299	259	0.03%	0.004%
12	3.174	579	586	589	rBV2	759	1005	0.11%	0.014%
13	3.358	636	643	646	rVB2	493	566	0.06%	0.008%
14	3.383	646	651	653	rBV2	321	352	0.04%	0.005%
15	3.573	706	710	713	rBV	233	159	0.02%	0.002%
16	3.657	732	736	739	rBV	240	199	0.02%	0.003%
17	3.933	817	822	827	rBV2	196	191	0.02%	0.003%
18	4.149	886	889	893	rBV2	236	180	0.02%	0.002%
19	4.322	940	943	948	rBV	321	356	0.04%	0.005%
20	4.361	951	955	958	rVV2	193	219	0.02%	0.003%
21	4.380	958	961	964	rVB	283	198	0.02%	0.003%
22	4.441	976	980	984	rVV	220	193	0.02%	0.003%
23	4.460	984	986	990	rVB	304	218	0.02%	0.003%
24	4.612	1023	1033	1069	rBV	59544	164161	17.26%	2.223%
25	4.978	1142	1147	1149	rBV2	274	275	0.03%	0.004%
26	5.055	1154	1171	1194	rBV	166380	374219	39.34%	5.067%
27	5.377	1267	1271	1278	rBV2	263	307	0.03%	0.004%
28	5.525	1314	1317	1320	rVB	223	176	0.02%	0.002%
29	5.595	1329	1339	1340	rBV2	241	315	0.03%	0.004%
30	5.718	1352	1377	1409	rBV2	342189	951281	100.00%	12.882%
31	6.113	1494	1500	1505	rBV3	366	422	0.04%	0.006%
32	6.145	1505	1510	1515	rBV2	309	293	0.03%	0.004%
33	6.242	1527	1540	1561	rBV	345915	665317	69.94%	9.009%
34	6.457	1604	1607	1611	rVB2	400	334	0.04%	0.005%
35	6.483	1613	1615	1618	rVV	242	163	0.02%	0.002%
36	6.528	1622	1629	1638	rVB4	1469	2614	0.27%	0.035%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
 Data File : VU057944.D
 Acq On : 23 Feb 2024 12:55
 Operator : MD/SY
 Sample : P1567-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

37	6.682	1663	1677	1706	rBV	217040	430936	45.30%	5.835%
38	6.914	1746	1749	1751	rBV	294	185	0.02%	0.003%
39	6.991	1770	1773	1775	rBV2	286	235	0.02%	0.003%
40	7.197	1828	1837	1840	rBV3	852	991	0.10%	0.013%
41	7.287	1862	1865	1873	rVB2	207	333	0.04%	0.005%
42	7.322	1873	1876	1881	rBV	213	227	0.02%	0.003%
43	7.402	1897	1901	1907	rVB2	141	170	0.02%	0.002%
44	7.438	1907	1912	1916	rVB2	189	238	0.03%	0.003%
45	7.460	1916	1919	1923	rBV2	258	222	0.02%	0.003%
46	7.560	1938	1950	1974	rBV	118682	217804	22.90%	2.949%
47	7.708	1991	1996	2001	rVV4	393	417	0.04%	0.006%
48	7.891	2040	2053	2083	rBV	419518	747278	78.55%	10.119%
49	8.174	2128	2141	2173	rBV	79858	143340	15.07%	1.941%
50	8.473	2232	2234	2239	rVB	224	176	0.02%	0.002%
51	8.544	2254	2256	2261	rVB3	301	236	0.02%	0.003%
52	8.579	2261	2267	2270	rVB2	250	290	0.03%	0.004%
53	8.627	2270	2282	2323	rBV3	185518	415255	43.65%	5.623%
54	8.849	2348	2351	2356	rBV3	315	283	0.03%	0.004%
55	8.936	2373	2378	2383	rVB2	197	249	0.03%	0.003%
56	8.968	2383	2388	2391	rBV2	214	197	0.02%	0.003%
57	9.052	2408	2414	2417	rBV2	191	231	0.02%	0.003%
58	9.119	2430	2435	2438	rBV	239	248	0.03%	0.003%
59	9.197	2455	2459	2462	rBV2	207	170	0.02%	0.002%
60	9.412	2514	2526	2562	rBV	485703	831308	87.39%	11.257%
61	9.566	2571	2574	2580	rVB2	342	395	0.04%	0.005%
62	9.640	2595	2597	2604	rVB2	277	295	0.03%	0.004%
63	9.952	2690	2694	2699	rVB2	276	277	0.03%	0.004%
64	10.113	2738	2744	2745	rBV	274	243	0.03%	0.003%
65	10.123	2745	2747	2753	rVV	373	321	0.03%	0.004%
66	10.222	2774	2778	2785	rVB2	268	352	0.04%	0.005%
67	10.489	2859	2861	2866	rVB2	371	222	0.02%	0.003%
68	10.750	2929	2942	2960	rBV	259073	427731	44.96%	5.792%
69	10.856	2971	2975	2980	rVB2	220	183	0.02%	0.002%
70	10.926	2994	2997	3000	rBV2	223	221	0.02%	0.003%
71	10.971	3008	3011	3013	rBV	212	184	0.02%	0.002%
72	11.097	3047	3050	3057	rVB2	304	248	0.03%	0.003%
73	11.229	3085	3091	3094	rBV	406	450	0.05%	0.006%
74	11.470	3159	3166	3169	rBV2	485	565	0.06%	0.008%
75	11.553	3186	3192	3195	rBV	208	277	0.03%	0.004%
76	11.592	3200	3204	3207	rBV2	249	257	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
 Data File : VU057944.D
 Acq On : 23 Feb 2024 12:55
 Operator : MD/SY
 Sample : P1567-19
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

77	11.647	3218	3221	3224	rBV	314	268	0.03%	0.004%
78	11.746	3248	3252	3259	rVB2	1016	1066	0.11%	0.014%
79	11.807	3259	3271	3300	rBV	492269	794466	83.52%	10.758%
80	12.187	3377	3389	3412	rBV	382781	637769	67.04%	8.636%
81	12.708	3548	3551	3553	rBV	272	180	0.02%	0.002%
82	12.769	3567	3570	3574	rVB	258	211	0.02%	0.003%
83	12.907	3608	3613	3615	rBV2	178	173	0.02%	0.002%
84	13.283	3727	3730	3732	rBV2	310	247	0.03%	0.003%
85	13.534	3806	3808	3811	rBV	284	220	0.02%	0.003%
86	13.663	3846	3848	3852	rVB2	288	164	0.02%	0.002%
87	13.692	3852	3857	3860	rBV	259	294	0.03%	0.004%
88	13.862	3904	3910	3916	rBV2	839	1285	0.14%	0.017%
89	13.926	3927	3930	3936	rVB2	379	357	0.04%	0.005%
90	13.997	3950	3952	3955	rBV	286	206	0.02%	0.003%
91	14.116	3983	3989	3990	rBV	451	376	0.04%	0.005%
92	14.200	4012	4015	4016	rBV	283	190	0.02%	0.003%
93	14.235	4024	4026	4029	rVB	390	223	0.02%	0.003%
94	14.257	4029	4033	4034	rBV	321	229	0.02%	0.003%
95	14.341	4055	4059	4065	rBV3	582	759	0.08%	0.010%
96	14.505	4105	4110	4112	rBV2	360	316	0.03%	0.004%
97	14.544	4119	4122	4125	rBV2	326	264	0.03%	0.004%
98	14.611	4141	4143	4146	rBV	287	206	0.02%	0.003%
99	14.855	4216	4219	4221	rBV	247	183	0.02%	0.002%
100	16.585	4755	4757	4760	rBV3	729	458	0.05%	0.006%




Sum of corrected areas: 7384772

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
Data File : VU057944.D
Acq On : 23 Feb 2024 12:55
Operator : MD/SY
Sample : P1567-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

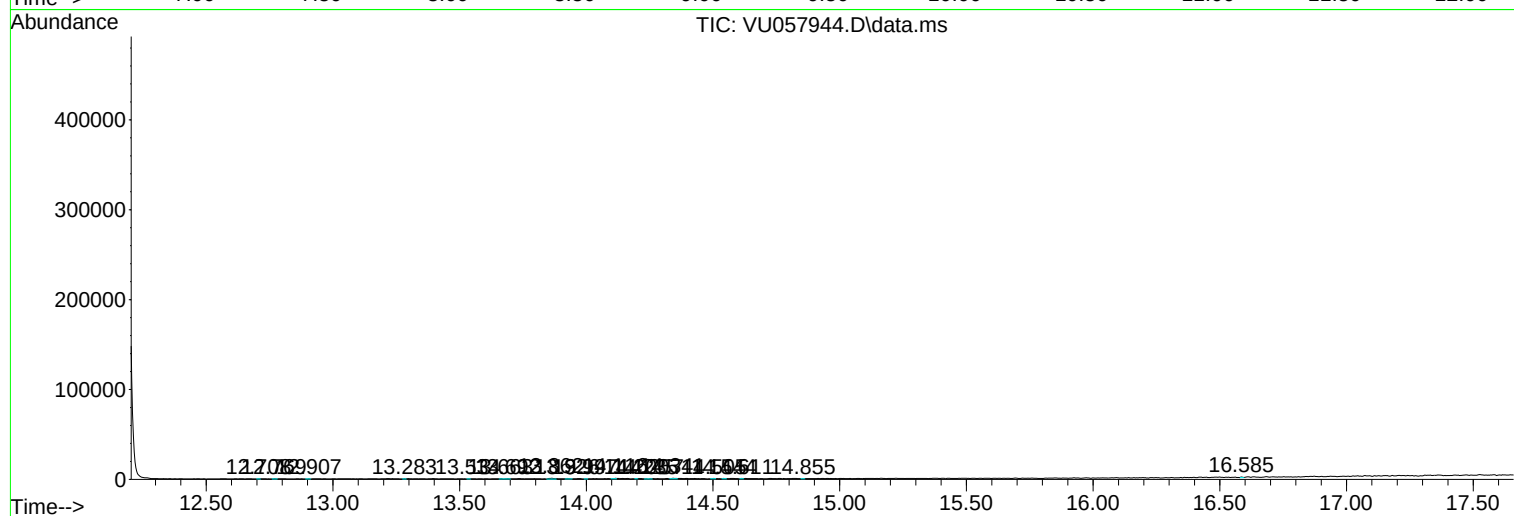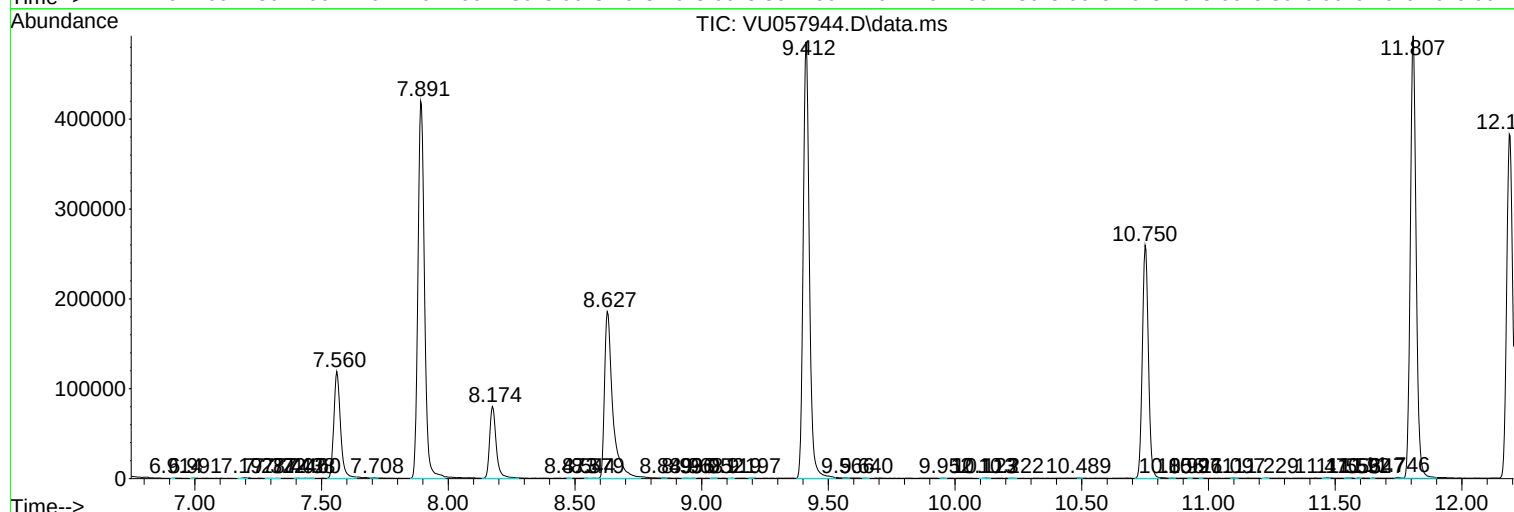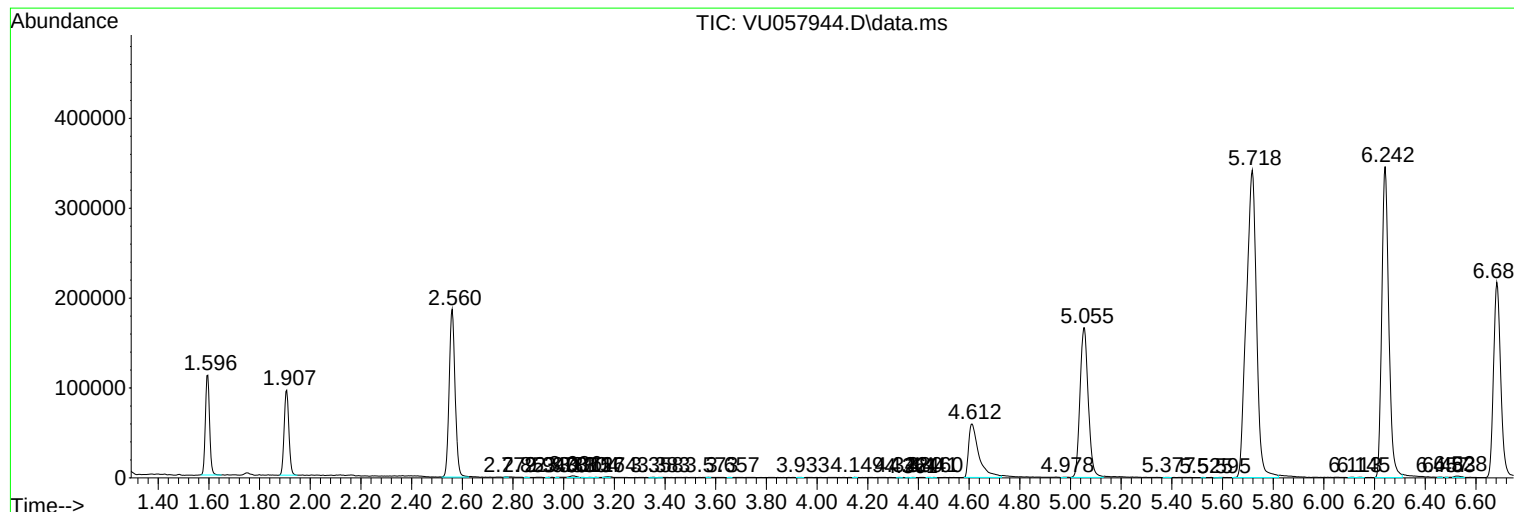

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
Data File : VU057944.D
Acq On : 23 Feb 2024 12:55
Operator : MD/SY
Sample : P1567-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
Data File : VU057944.D
Acq On : 23 Feb 2024 12:55
Operator : MD/SY
Sample : P1567-19
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------