


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022324\
Data File : VU057938.D
Acq On : 23 Feb 2024 08:59
Operator : MD/SY
Sample : BFB043
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB043

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Title : VOC Analysis
Last Update : Fri Feb 23 23:00:11 2024

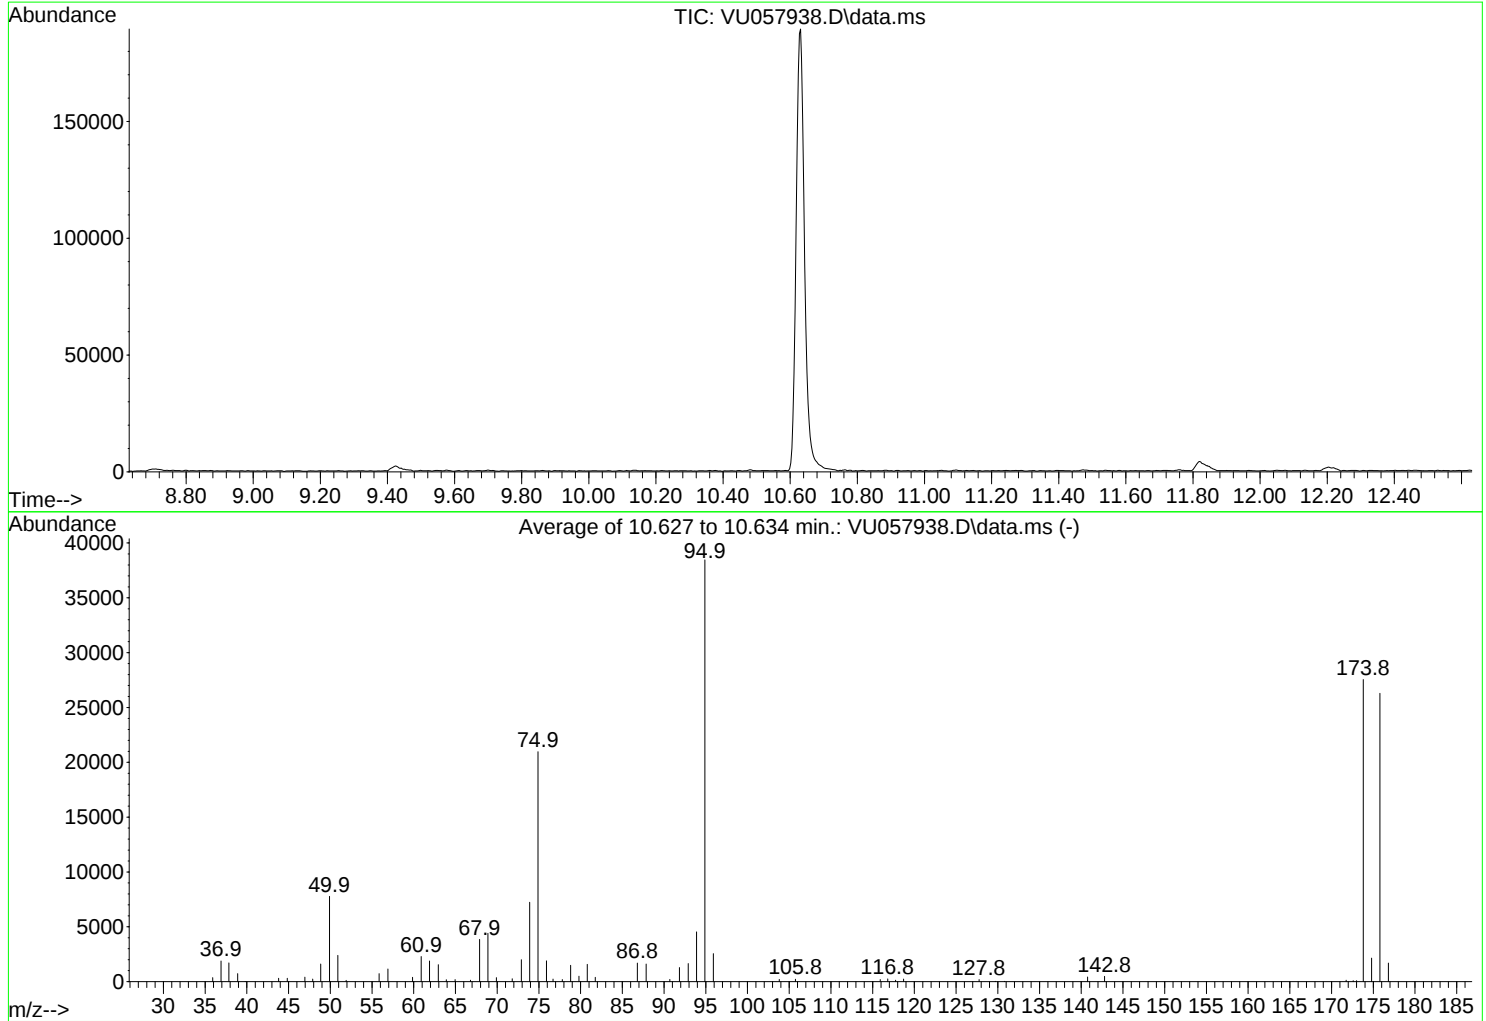

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	7772	PASS
75	95	30	80	54.5	20968	PASS
95	95	100	100	100.0	38464	PASS
96	95	5	9	6.6	2557	PASS
173	174	0.00	2	0.3	86	PASS
174	95	50	120	71.6	27547	PASS
175	174	5	9	7.8	2148	PASS
176	174	95	101	95.5	26296	PASS
177	176	5	9	6.4	1691	PASS

m/z	Abundance
39.90	148.0
43.80	417.0

Instrument :
MSVOA_U
ClientSampleId :
BFB043

m/z	Abundance
35.90	396.0
36.90	2016.0
37.90	1788.0
38.90	704.0
39.80	173.0
43.90	702.0
44.80	291.0
47.00	429.0
47.90	200.0
48.90	1596.0
49.90	8137.0
50.90	2340.0
51.90	107.0
55.80	748.0
56.90	1234.0
59.90	462.0
60.90	2285.0
61.90	2053.0
62.90	1602.0
63.90	169.0
65.00	199.0
66.80	117.0
67.90	3970.0
68.90	4615.0
69.90	357.0
71.80	271.0
72.90	1916.0
73.90	7231.0
74.90	21632.0
75.90	2081.0
76.70	175.0
77.80	230.0
78.80	1509.0
79.80	432.0
80.80	1628.0
81.80	400.0
86.80	1803.0
87.90	1584.0
90.70	240.0
91.80	1307.0
92.90	1725.0
93.90	4546.0
94.90	39024.0
95.90	2606.0
103.80	207.0
105.70	234.0
115.90	163.0
116.80	209.0
117.80	151.0
118.70	274.0
127.80	185.0
129.70	102.0
140.70	432.0
142.80	459.0
171.70	123.0
173.00	259.0
173.80	27712.0
174.80	2045.0
175.80	26240.0
176.80	1758.0

Instrument :
MSVOA_U
ClientSampleId :
BFB043

m/z	Abundance
35.90	381.0
36.90	1929.0
37.90	1754.0
38.90	759.0
39.80	167.0
43.80	748.0
44.90	308.0
46.90	438.0
47.90	231.0
48.90	1594.0
49.90	7922.0
50.90	2425.0
51.90	121.0
55.90	742.0
56.90	1178.0
59.80	403.0
60.90	2419.0
61.90	1914.0
63.00	1567.0
63.90	181.0
65.00	206.0
66.80	141.0
67.90	3954.0
68.90	4489.0
69.90	385.0
71.80	277.0
72.90	2106.0
73.90	7391.0
74.90	21424.0
75.90	1926.0
76.70	247.0
77.80	208.0
78.80	1528.0
79.80	515.0
80.80	1595.0
81.80	390.0
86.80	1749.0
87.90	1649.0
90.70	198.0
91.80	1356.0
92.90	1671.0
93.90	4685.0
94.90	39400.0
95.90	2596.0
103.80	218.0
105.80	229.0
115.90	201.0
116.80	251.0
117.80	144.0
118.70	252.0
127.80	219.0
130.80	105.0
140.70	426.0
142.80	501.0
171.80	141.0
172.60	140.0
173.80	28408.0
174.80	2249.0
175.80	27088.0
176.80	1726.0

Instrument :
MSVOA_U
ClientSampleId :
BFB043

m/z	Abundance
35.90	323.0
36.90	1696.0
37.80	1599.0
38.90	731.0
39.80	156.0
43.80	726.0
44.90	308.0
46.90	378.0
47.90	257.0
48.80	1620.0
49.90	7257.0
50.90	2400.0
51.90	112.0
55.90	685.0
56.90	1051.0
59.80	316.0
60.90	2187.0
61.90	1669.0
63.00	1485.0
63.90	175.0
64.90	170.0
66.80	138.0
67.90	3625.0
68.90	4101.0
69.90	371.0
71.80	260.0
72.90	1987.0
73.90	7075.0
74.90	19848.0
75.90	1700.0
76.70	272.0
77.80	147.0
78.80	1443.0
79.80	535.0
80.80	1486.0
81.70	377.0
86.80	1509.0
87.80	1582.0
90.70	166.0
91.90	1196.0
92.90	1575.0
93.90	4387.0
94.90	36968.0
95.90	2470.0
103.80	211.0
105.80	216.0
115.90	197.0
116.80	270.0
117.70	123.0
118.70	190.0
127.70	184.0
140.80	413.0
142.80	478.0
171.80	149.0
172.60	133.0
173.80	26520.0
174.80	2151.0
175.80	25560.0
176.80	1590.0

Instrument :
MSVOA_U
ClientSampleId :
BFB043