




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047267.D
 Acq On : 25 Feb 2022 12:23
 Operator : SY/MD
 Sample : N1667-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBRL2

Manual IntegrationsAPPROVED

Quant Time: Feb 28 02:02:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Feb 28 02:01:00 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 02/28/2022
 Supervised By :Mahesh Dadoda 03/01/2022

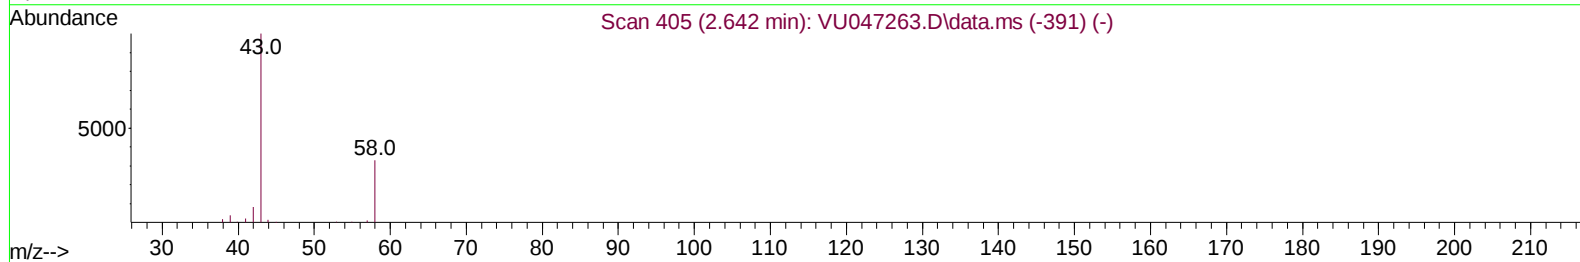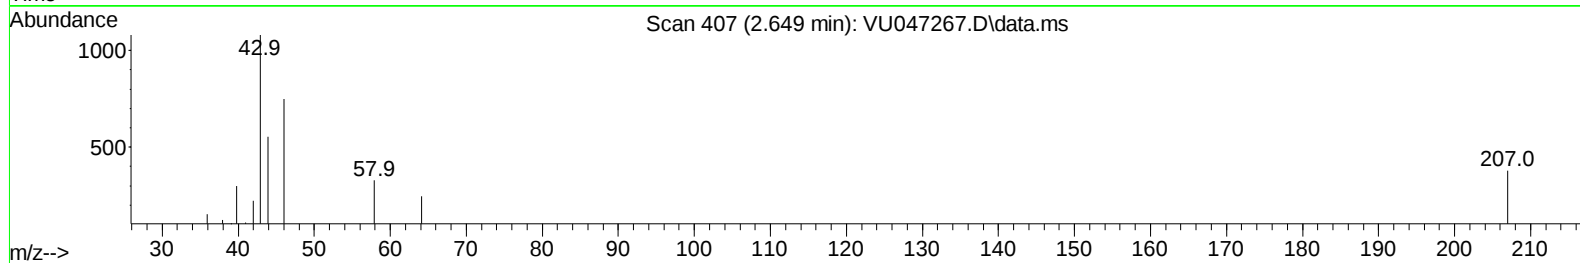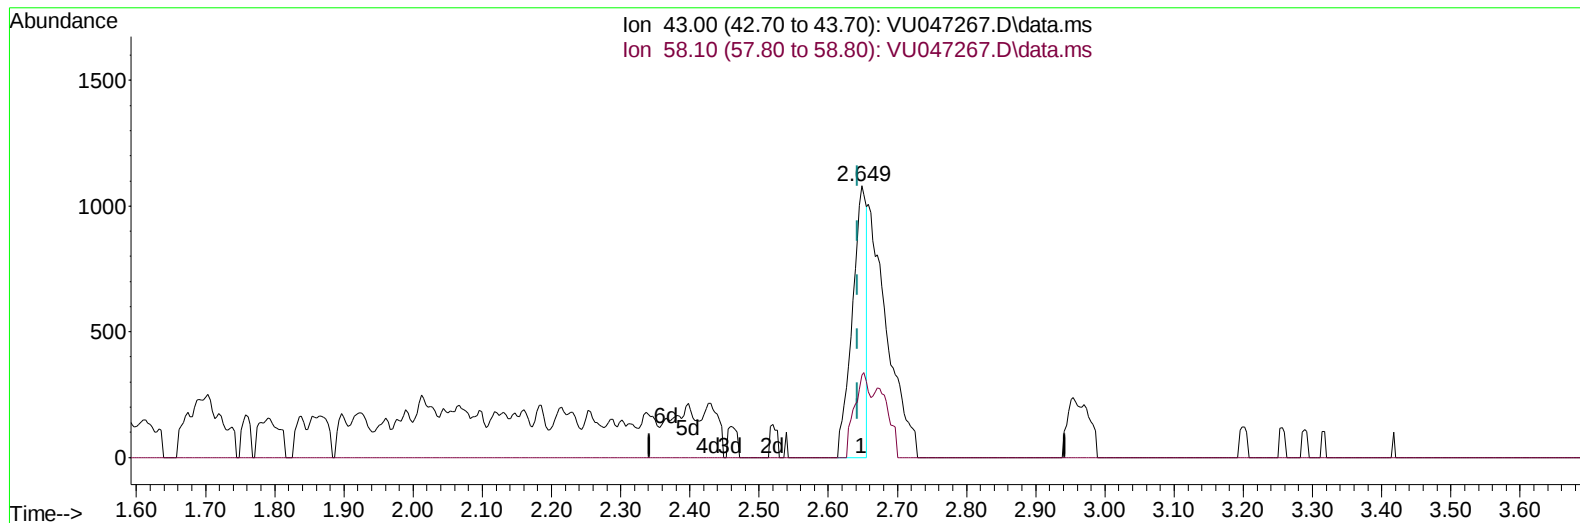

TIC: VU047267.D\data.ms

(13) Acetone (T)

2.649min (+ 0.006) 2.16 ug/L

response 1535

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	35.50	33.03
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047267.D
 Acq On : 25 Feb 2022 12:23
 Operator : SY/MD
 Sample : N1667-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBRL2

Manual IntegrationsAPPROVED

Quant Time: Feb 28 02:02:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Feb 28 02:01:00 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 02/28/2022
 Supervised By :Mahesh Dadoda 03/01/2022

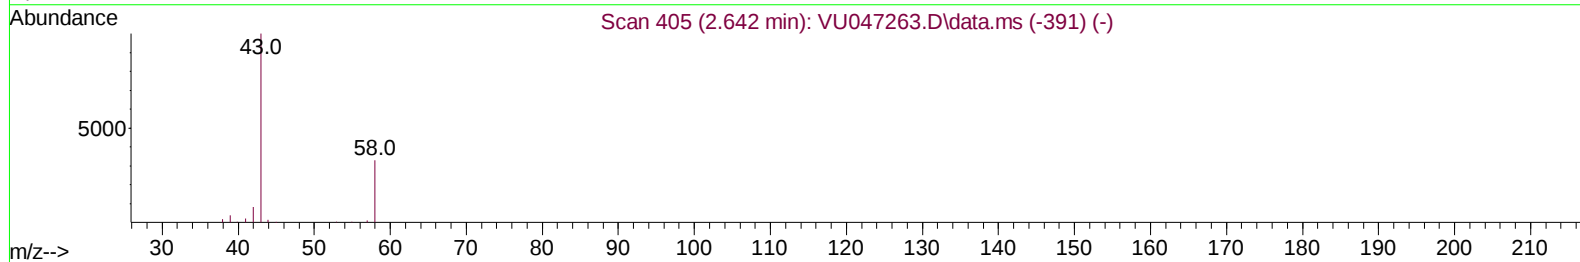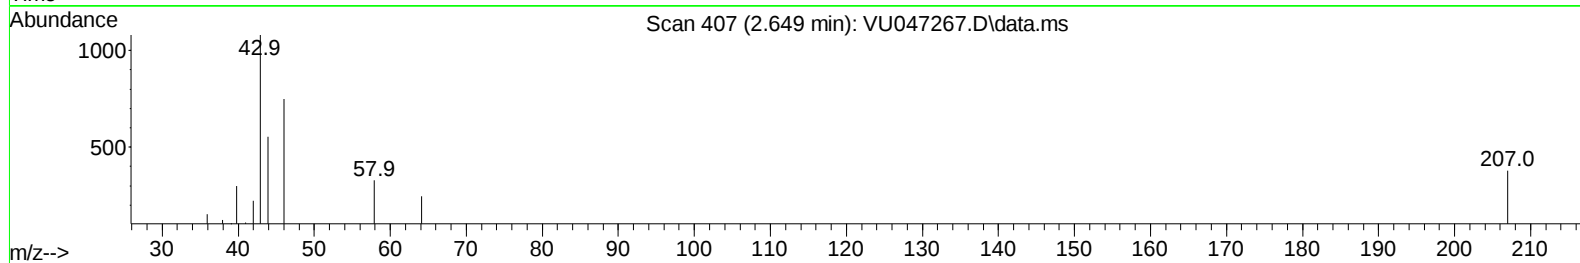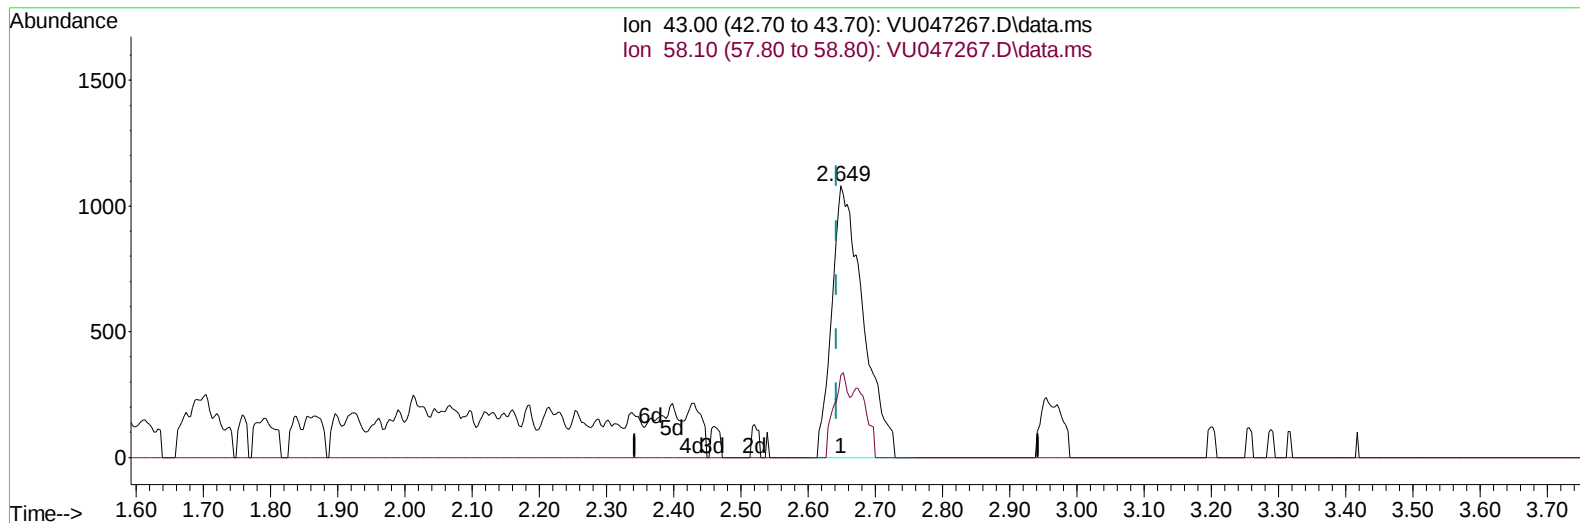

TIC: VU047267.D\data.ms

(13) Acetone (T)

2.649min (+ 0.006) 4.90 ug/L m

response 3486

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	35.50	14.54
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047267.D
 Acq On : 25 Feb 2022 12:23
 Operator : SY/MD
 Sample : N1667-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBRL2

Manual IntegrationsAPPROVED

Quant Time: Feb 28 02:02:02 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Feb 28 02:01:00 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 02/28/2022
 Supervised By :Mahesh Dadoda 03/01/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	138787	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	134357	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	77791	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	106713	84.661	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135	Recovery	=	169.320%#	
7) Chloroethane-d5	1.919	69	87198	93.321	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130	Recovery	=	186.640%#	
11) 1,1-Dichloroethene-d2	2.575	63	146696	70.230	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	140.460%#	
21) 2-Butanone-d5	4.636	46	199787	204.372	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130	Recovery	=	204.370%#	
24) Chloroform-d	5.066	84	187934	91.842	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	183.680%#	
26) 1,2-Dichloroethane-d4	5.706	65	120252	91.558	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	183.120%#	
32) Benzene-d6	5.732	84	398695	89.258	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125	Recovery	=	178.520%#	
36) 1,2-Dichloropropane-d6	6.693	67	122121	84.305	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120	Recovery	=	168.620%#	
41) Toluene-d8	7.899	98	372952	87.693	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	175.380%#	
43) trans-1,3-Dichloroprop...	8.179	79	59271	78.079	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125	Recovery	=	156.160%#	
47) 2-Hexanone-d5	8.635	63	157027	189.219	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130	Recovery	=	189.220%#	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	181310	85.840	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120	Recovery	=	171.680%#	
66) 1,2-Dichlorobenzene-d4	12.195	152	151127	81.914	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120	Recovery	=	163.820%#	
Target Compounds						
13) Acetone	2.649	43	3486m	4.895	ug/L	
42) Toluene	7.970	91	7622	1.656	ug/L	96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
Data File : VU047267.D
Acq On : 25 Feb 2022 12:23
Operator : SY/MD
Sample : N1667-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBRL2

Manual IntegrationsAPPROVED

Quant Time: Feb 28 02:02:02 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Feb 28 02:01:00 2022
Response via : Initial Calibration

Reviewed By :John Carlone 02/28/2022
Supervised By :Mahesh Dadoda 03/01/2022

