




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047271.D
 Acq On : 25 Feb 2022 15:16
 Operator : SY/MD
 Sample : N1667-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBRL0

Manual IntegrationsAPPROVED

Quant Time: Feb 28 02:02:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Feb 28 02:01:00 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 02/28/2022
 Supervised By :Mahesh Dadoda 03/01/2022

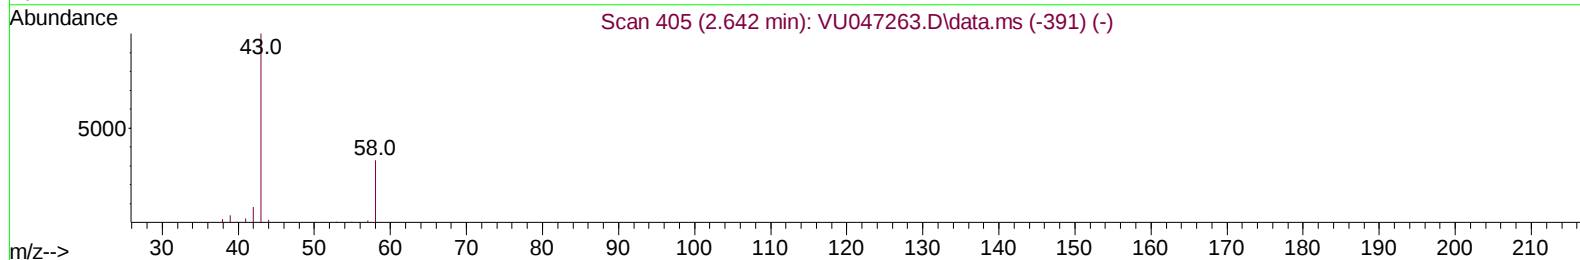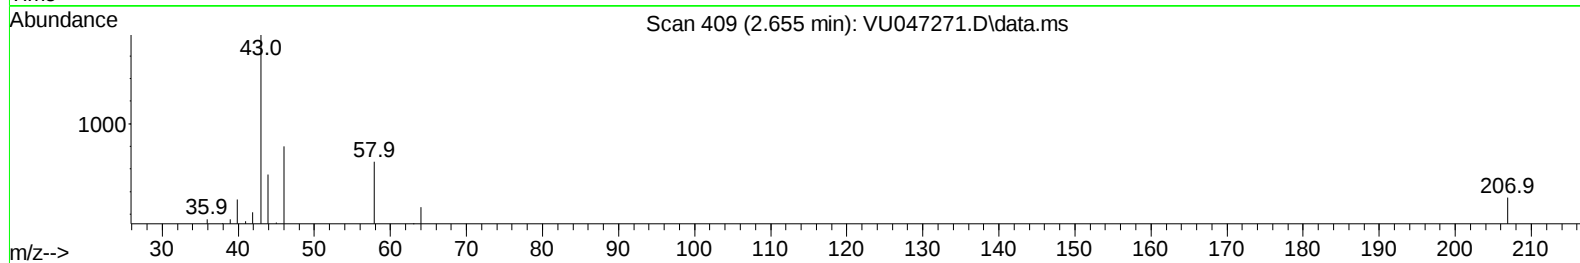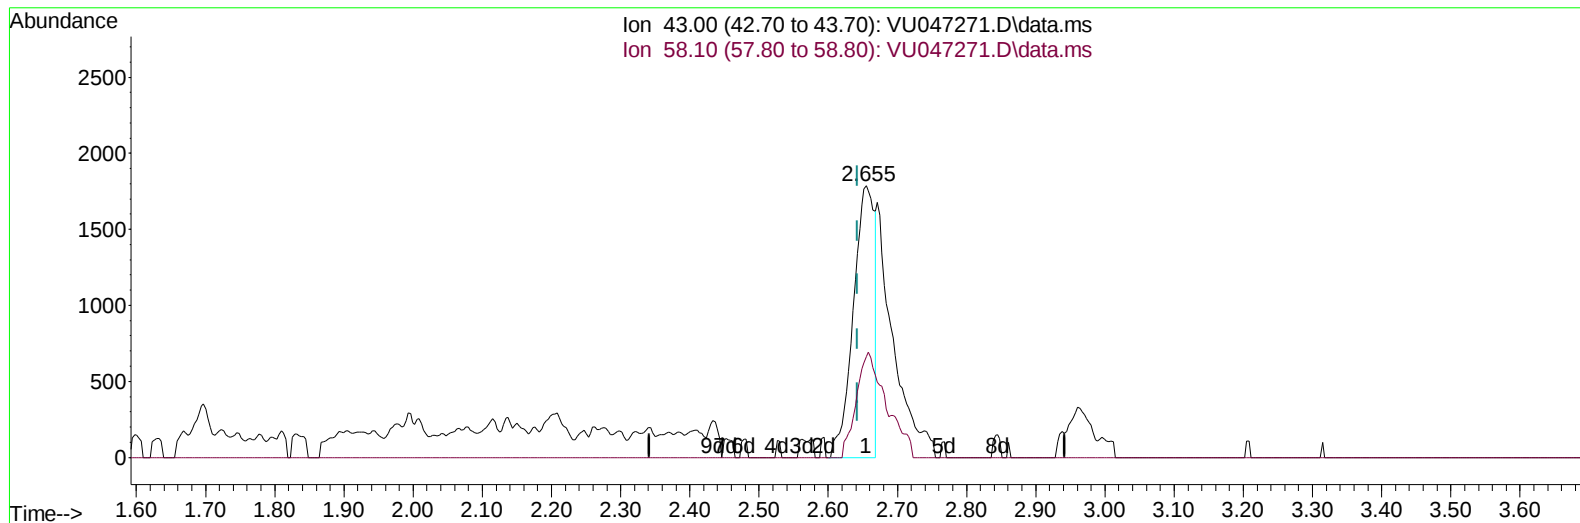

TIC: VU047271.D\data.ms

(13) Acetone (T)

2.655min (+ 0.013) 2.01 ug/L

response 3800

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	35.50	45.24
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047271.D
 Acq On : 25 Feb 2022 15:16
 Operator : SY/MD
 Sample : N1667-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBRL0

Manual IntegrationsAPPROVED

Quant Time: Feb 28 02:02:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Feb 28 02:01:00 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 02/28/2022
 Supervised By :Mahesh Dadoda 03/01/2022

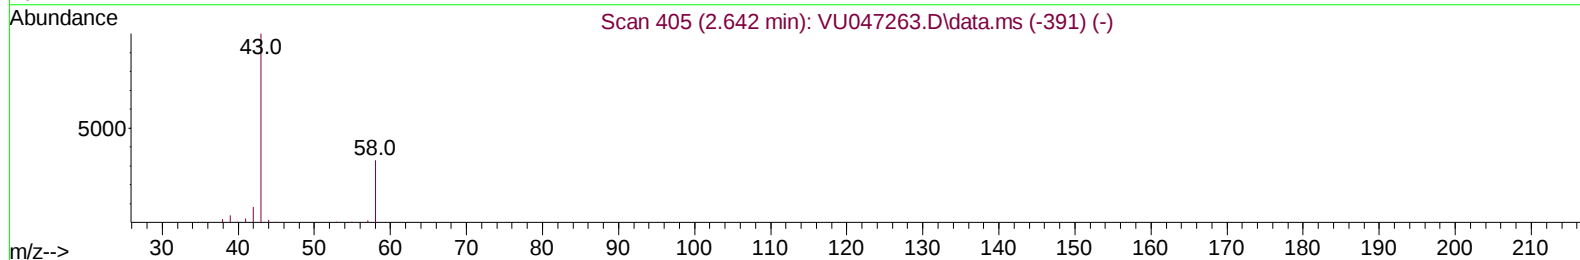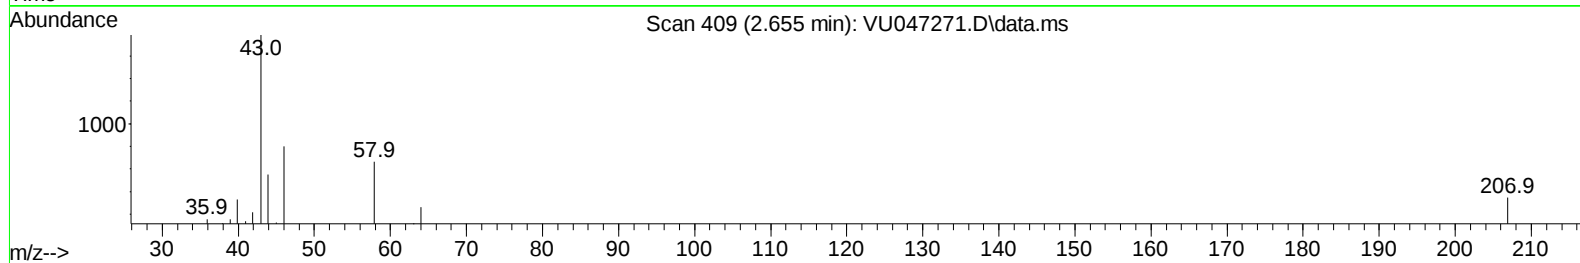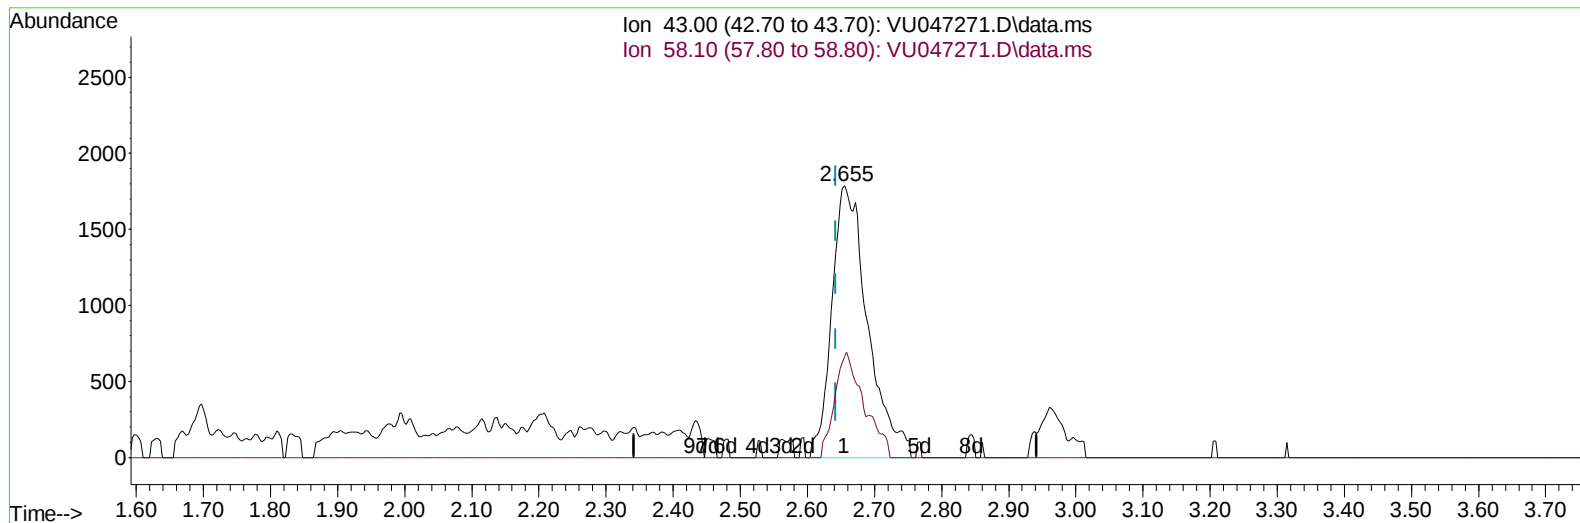

TIC: VU047271.D\data.ms

(13) Acetone (T)

2.655min (+ 0.013) 3.50 ug/L m

response 6604

Ion	Exp%	Act%
43.00	100.00	100.00
58.10	35.50	26.03
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047271.D
 Acq On : 25 Feb 2022 15:16
 Operator : SY/MD
 Sample : N1667-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBRL0

Manual IntegrationsAPPROVED

Quant Time: Feb 28 02:02:53 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Feb 28 02:01:00 2022
 Response via : Initial Calibration

Reviewed By : John Carlone 02/28/2022
 Supervised By : Mahesh Dadoda 03/01/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.253	114		367643	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117		357754	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152		208278	50.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.604	65		137242	41.103	ug/L	0.00
Spiked Amount 50.000	Range 60	- 135		Recovery	=	82.200%	
7) Chloroethane-d5	1.919	69		111992	45.246	ug/L	0.00
Spiked Amount 50.000	Range 70	- 130		Recovery	=	90.500%	
11) 1,1-Dichloroethene-d2	2.571	63		189343	34.220	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	68.440%	
21) 2-Butanone-d5	4.639	46		257179	99.314	ug/L	0.00
Spiked Amount 100.000	Range 40	- 130		Recovery	=	99.310%	
24) Chloroform-d	5.067	84		243819	44.981	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	89.960%	
26) 1,2-Dichloroethane-d4	5.706	65		156963	45.115	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	90.240%	
32) Benzene-d6	5.732	84		513822	43.201	ug/L	0.00
Spiked Amount 50.000	Range 70	- 125		Recovery	=	86.400%	
36) 1,2-Dichloropropane-d6	6.694	67		159396	41.325	ug/L	0.00
Spiked Amount 50.000	Range 70	- 120		Recovery	=	82.660%	
41) Toluene-d8	7.899	98		490663	43.328	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	86.660%	
43) trans-1,3-Dichloroprop...	8.182	79		78384	38.779	ug/L	0.00
Spiked Amount 50.000	Range 60	- 125		Recovery	=	77.560%	
47) 2-Hexanone-d5	8.636	63		204702	92.638	ug/L	0.00
Spiked Amount 100.000	Range 45	- 130		Recovery	=	92.640%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84		240519	42.766	ug/L	0.00
Spiked Amount 50.000	Range 65	- 120		Recovery	=	85.540%	
66) 1,2-Dichlorobenzene-d4	12.195	152		202937	41.083	ug/L	0.00
Spiked Amount 50.000	Range 80	- 120		Recovery	=	82.160%	
Target Compounds							
13) Acetone	2.655	43		6604m	3.501	ug/L	Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
Data File : VU047271.D
Acq On : 25 Feb 2022 15:16
Operator : SY/MD
Sample : N1667-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBRL0

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 02/28/2022
Supervised By : Mahesh Dadoda 03/01/2022

Quant Time: Feb 28 02:02:53 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Feb 28 02:01:00 2022
Response via : Initial Calibration

