

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047272.D
 Acq On : 25 Feb 2022 15:39
 Operator : SY/MD
 Sample : N1667-03
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Quant Time: Feb 28 02:03:04 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Mon Feb 28 02:01:00 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.250	114	354528	50.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117	343684	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	202824	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	132483	41.146	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	=	82.300%	
7) Chloroethane-d5	1.919	69	110044	46.104	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	=	92.200%	
11) 1,1-Dichloroethene-d2	2.572	63	182452	34.194	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	68.380%	
21) 2-Butanone-d5	4.633	46	260256	104.221	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	=	104.220%	
24) Chloroform-d	5.067	84	236335	45.213	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	90.420%	
26) 1,2-Dichloroethane-d4	5.707	65	152814	45.548	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	91.100%	
32) Benzene-d6	5.729	84	499087	43.680	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	=	87.360%	
36) 1,2-Dichloropropane-d6	6.694	67	155209	41.887	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	=	83.780%	
41) Toluene-d8	7.899	98	472746	43.455	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	86.920%	
43) trans-1,3-Dichloroprop...	8.179	79	77218	39.766	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	=	79.540%	
47) 2-Hexanone-d5	8.632	63	207258	97.634	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	=	97.630%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84	239074	44.249	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	=	88.500%	
66) 1,2-Dichlorobenzene-d4	12.192	152	199602	41.495	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	=	82.980%	
Target Compounds					Qvalue	
13) Acetone	2.649	43	6566	3.609	ug/L	95


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
Data File : VU047272.D
Acq On : 25 Feb 2022 15:39
Operator : SY/MD
Sample : N1667-03
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001


Quant Time: Feb 28 02:03:04 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis
QLast Update : Mon Feb 28 02:01:00 2022
Response via : Initial Calibration

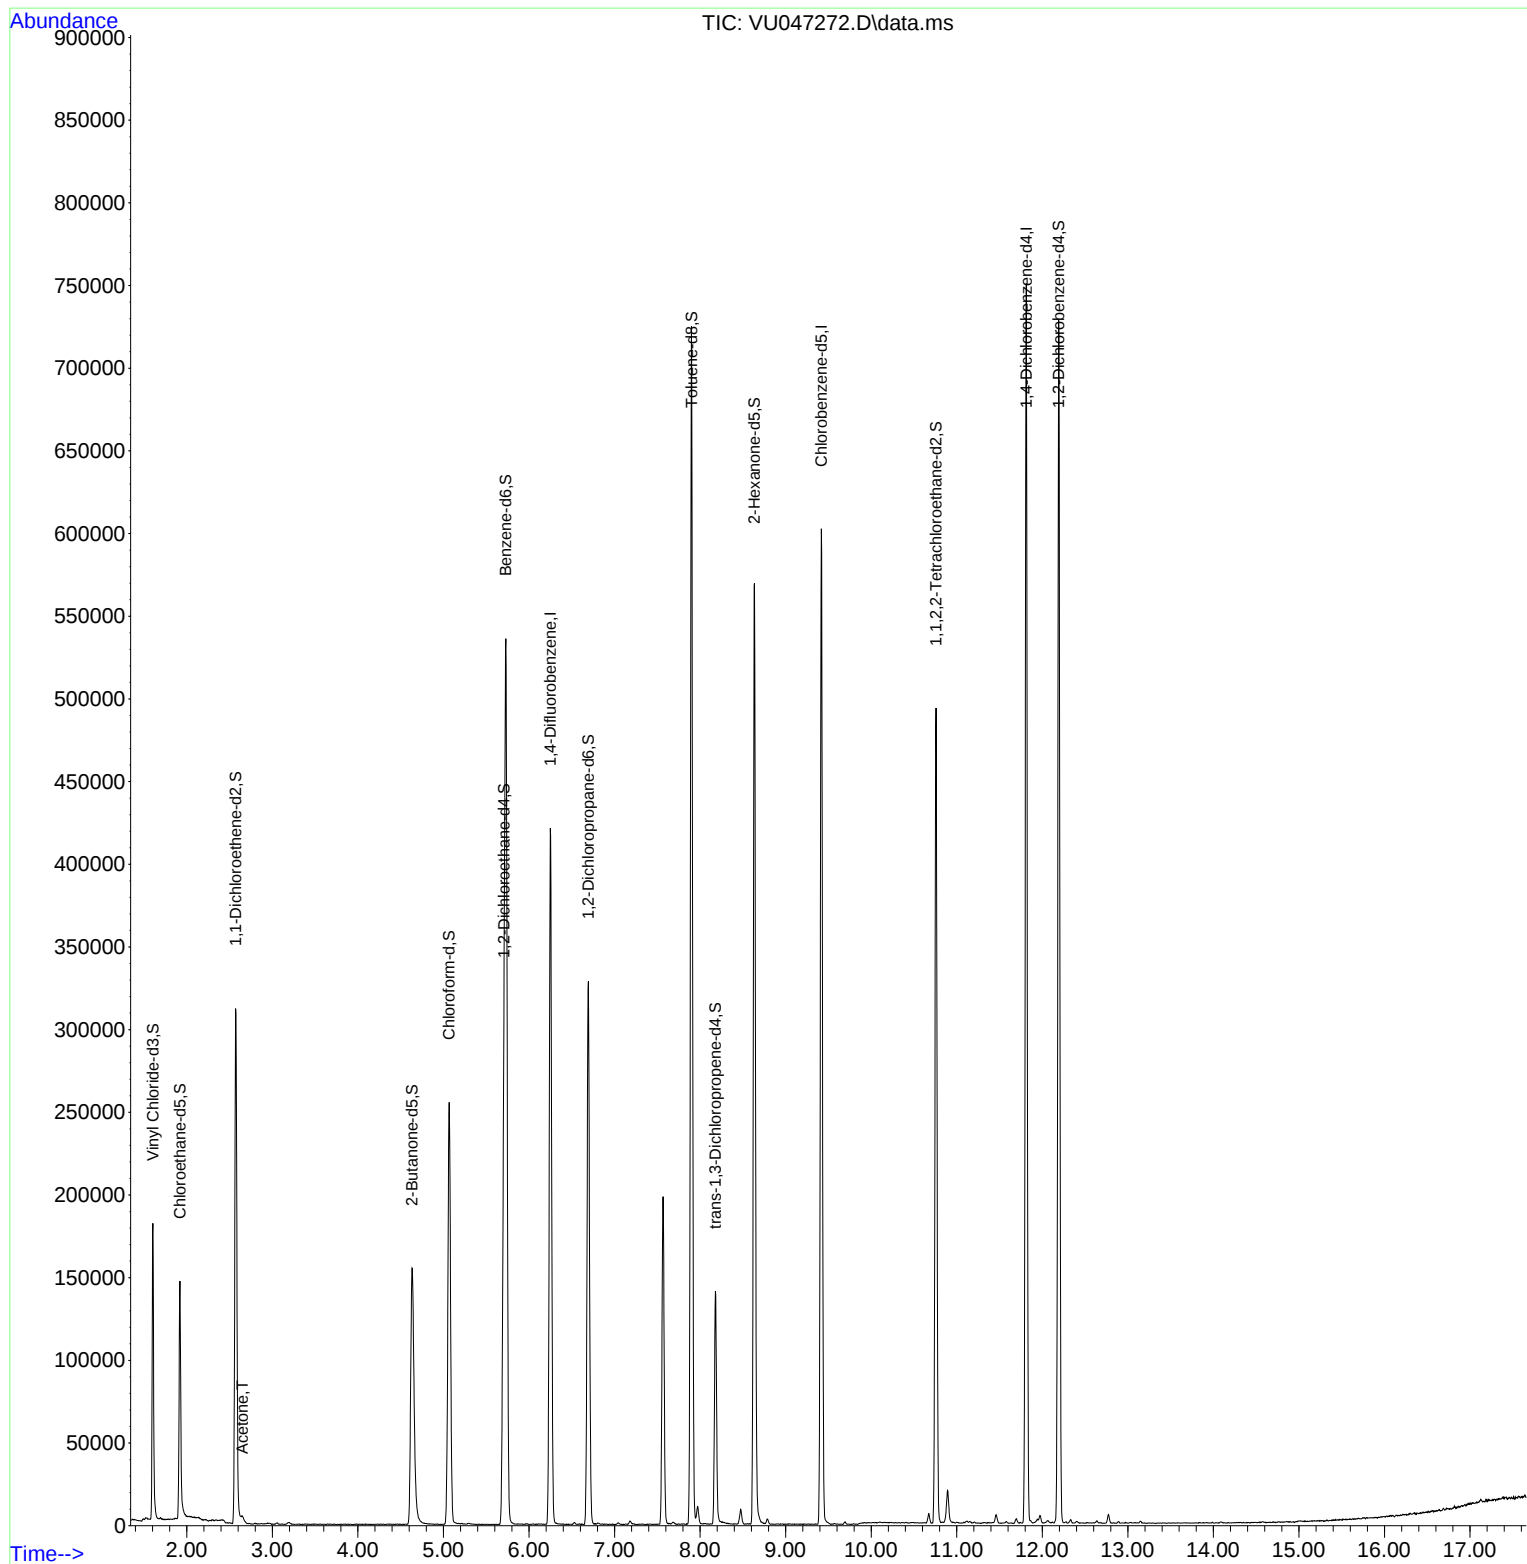

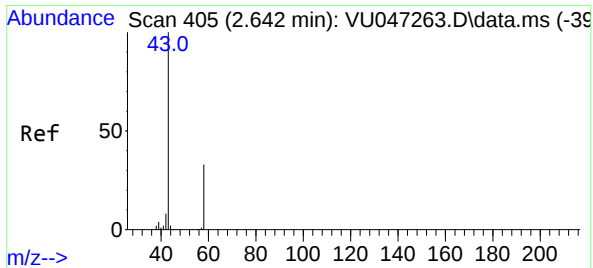

#13
Acetone
Concen: 3.609 ug/L
RT: 2.649 min Scan# 40
Delta R.T. 0.007 min
Lab File: VU047272.D
Acq: 25 Feb 2022 15:39

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

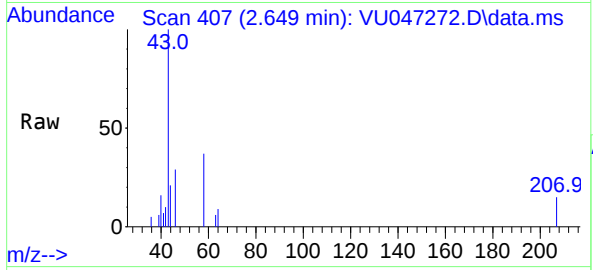

Tgt Ion: 43 Resp: 6566
Ion Ratio Lower Upper
43 100
58 32.7 0.0 71.0

