

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047265.D
 Acq On : 25 Feb 2022 11:36
 Operator : SY/MD
 Sample : VU0225WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK071

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M

Title : VOC Analysis

Signal : TIC: VU047265.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	102	rBV	190116	226660	15.13%	1.858%
2	1.919	171	180	206	rBV	146239	204049	13.62%	1.673%
3	2.575	371	384	418	rBV	329524	559143	37.32%	4.585%
4	3.057	526	534	538	rVB4	597	825	0.06%	0.007%
5	3.189	571	575	577	rBV2	304	245	0.02%	0.002%
6	3.295	604	608	614	rBV2	213	230	0.02%	0.002%
7	3.350	623	625	630	rVB2	241	166	0.01%	0.001%
8	3.395	636	639	645	rVB	228	190	0.01%	0.002%
9	3.565	687	692	698	rBV2	224	255	0.02%	0.002%
10	3.678	723	727	733	rVB2	201	176	0.01%	0.001%
11	3.733	740	744	749	rBV3	211	254	0.02%	0.002%
12	3.845	776	779	784	rBV2	155	134	0.01%	0.001%
13	3.954	810	813	816	rVV2	236	142	0.01%	0.001%
14	3.977	816	820	822	rBV2	270	173	0.01%	0.001%
15	4.167	874	879	882	rBV2	186	180	0.01%	0.001%
16	4.276	909	913	916	rBV	173	133	0.01%	0.001%
17	4.318	922	926	930	rBV	320	290	0.02%	0.002%
18	4.363	935	940	942	rBV	195	157	0.01%	0.001%
19	4.424	955	959	962	rBV3	203	157	0.01%	0.001%
20	4.478	972	976	977	rBV2	241	125	0.01%	0.001%
21	4.642	1010	1027	1075	rBV	136496	455678	30.41%	3.736%
22	4.906	1107	1109	1113	rVB2	278	131	0.01%	0.001%
23	5.003	1135	1139	1142	rBV	206	180	0.01%	0.001%
24	5.067	1142	1159	1186	rVV	265043	581103	38.78%	4.765%
25	5.401	1260	1263	1269	rVB	195	127	0.01%	0.001%
26	5.472	1279	1285	1290	rVB2	183	195	0.01%	0.002%
27	5.498	1290	1293	1295	rBV2	159	124	0.01%	0.001%
28	5.546	1302	1308	1311	rVB2	183	174	0.01%	0.001%
29	5.626	1329	1333	1339	rVB3	158	192	0.01%	0.002%
30	5.729	1339	1365	1395	rBV2	566139	1498308	100.00%	12.285%
31	5.848	1400	1402	1410	rVB3	331	300	0.02%	0.002%
32	5.916	1419	1423	1427	rBV3	289	314	0.02%	0.003%
33	5.977	1438	1442	1448	rVB2	446	503	0.03%	0.004%
34	6.009	1448	1452	1455	rBV2	269	190	0.01%	0.002%
35	6.035	1455	1460	1462	rBV4	363	296	0.02%	0.002%
36	6.102	1479	1481	1483	rVV2	379	192	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047265.D
 Acq On : 25 Feb 2022 11:36
 Operator : SY/MD
 Sample : VU0225WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK071

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	6.112	1483	1484	1492	rVB4	413	462	0.03%	0.004%
38	6.150	1492	1496	1504	rBV2	268	386	0.03%	0.003%
39	6.253	1512	1528	1547	rBV	406553	770814	51.45%	6.320%
40	6.408	1574	1576	1580	rVB2	159	131	0.01%	0.001%
41	6.533	1605	1615	1623	rVB5	1499	2520	0.17%	0.021%
42	6.597	1633	1635	1640	rVB3	248	196	0.01%	0.002%
43	6.694	1650	1665	1691	rVB	339947	663910	44.31%	5.444%
44	6.810	1696	1701	1705	rVV4	776	905	0.06%	0.007%
45	6.835	1707	1709	1712	rVB2	365	198	0.01%	0.002%
46	6.957	1744	1747	1754	rVB3	220	260	0.02%	0.002%
47	7.009	1754	1763	1764	rBV2	283	223	0.01%	0.002%
48	7.041	1770	1773	1774	rBV	377	213	0.01%	0.002%
49	7.186	1810	1818	1826	rVB2	2025	3229	0.22%	0.026%
50	7.282	1843	1848	1852	rBV3	154	218	0.01%	0.002%
51	7.324	1855	1861	1862	rBV2	274	187	0.01%	0.002%
52	7.437	1893	1896	1899	rBV2	251	170	0.01%	0.001%
53	7.488	1909	1912	1918	rVB3	161	135	0.01%	0.001%
54	7.568	1923	1937	1955	rBV	209918	365805	24.41%	2.999%
55	7.655	1962	1964	1965	rVV	372	180	0.01%	0.001%
56	7.681	1965	1972	1986	rVB7	1464	2845	0.19%	0.023%
57	7.755	1992	1995	1997	rVB3	233	135	0.01%	0.001%
58	7.790	2002	2006	2008	rBV3	226	185	0.01%	0.002%
59	7.835	2017	2020	2025	rVB3	235	188	0.01%	0.002%
60	7.900	2025	2040	2055	rBV	754815	1283340	85.65%	10.523%
61	7.970	2056	2062	2074	rVB	10628	17329	1.16%	0.142%
62	8.047	2082	2086	2093	rBV4	327	367	0.02%	0.003%
63	8.076	2093	2095	2099	rVB2	275	176	0.01%	0.001%
64	8.182	2108	2128	2150	rBV	146481	251123	16.76%	2.059%
65	8.388	2188	2192	2195	rBV4	502	419	0.03%	0.003%
66	8.420	2199	2202	2204	rVB3	265	168	0.01%	0.001%
67	8.472	2211	2218	2231	rVB2	4479	8581	0.57%	0.070%
68	8.552	2241	2243	2245	rBV2	213	133	0.01%	0.001%
69	8.636	2255	2269	2295	rBV	595877	1020944	68.14%	8.371%
70	8.880	2342	2345	2348	rVB2	340	153	0.01%	0.001%
71	8.899	2348	2351	2354	rBV2	316	229	0.02%	0.002%
72	8.925	2354	2359	2363	rVV2	587	696	0.05%	0.006%
73	8.957	2367	2369	2373	rVV	323	189	0.01%	0.002%
74	8.980	2373	2376	2379	rVV3	202	174	0.01%	0.001%
75	8.993	2379	2380	2385	rVB2	291	193	0.01%	0.002%
76	9.067	2398	2403	2407	rVB4	385	313	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047265.D
 Acq On : 25 Feb 2022 11:36
 Operator : SY/MD
 Sample : VU0225WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK071

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

77	9.154	2426	2430	2434	rVB3	237	168	0.01%	0.001%
78	9.173	2434	2436	2438	rBV	254	138	0.01%	0.001%
79	9.227	2449	2453	2456	rBV2	239	190	0.01%	0.002%
80	9.330	2480	2485	2486	rVV	302	251	0.02%	0.002%
81	9.350	2489	2491	2497	rVB4	259	198	0.01%	0.002%
82	9.417	2497	2512	2549	rBV	599392	982359	65.56%	8.055%
83	9.690	2590	2597	2606	rBV4	1322	1947	0.13%	0.016%
84	9.784	2622	2626	2627	rBV2	462	335	0.02%	0.003%
85	10.671	2896	2902	2911	rVB	7953	11259	0.75%	0.092%
86	10.758	2916	2929	2949	rBV	520545	830719	55.44%	6.811%
87	11.414	3129	3133	3138	rBV4	764	758	0.05%	0.006%
88	11.462	3138	3148	3161	rVB5	5751	9986	0.67%	0.082%
89	11.578	3180	3184	3194	rVB4	1338	2121	0.14%	0.017%
90	11.697	3213	3221	3229	rBV3	3467	5254	0.35%	0.043%
91	11.813	3244	3257	3272	rBV	739741	1156250	77.17%	9.481%
92	11.944	3292	3298	3302	rBV5	1953	2887	0.19%	0.024%
93	11.973	3302	3307	3317	rVB2	5204	7270	0.49%	0.060%
94	12.038	3323	3327	3330	rBV3	509	434	0.03%	0.004%
95	12.195	3359	3376	3391	rBV	772635	1241986	82.89%	10.184%
96	12.327	3409	3417	3426	rBV6	2186	3513	0.23%	0.029%
97	12.407	3432	3442	3445	rBV5	1076	1660	0.11%	0.014%
98	12.636	3511	3513	3519	rVB5	938	996	0.07%	0.008%
99	12.771	3551	3555	3568	rVB4	2129	3460	0.23%	0.028%
100	13.150	3666	3673	3686	rVB7	1192	2158	0.14%	0.018%


Sum of corrected areas: 12196010

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
Data File : VU047265.D
Acq On : 25 Feb 2022 11:36
Operator : SY/MD
Sample : VU0225WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK071

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

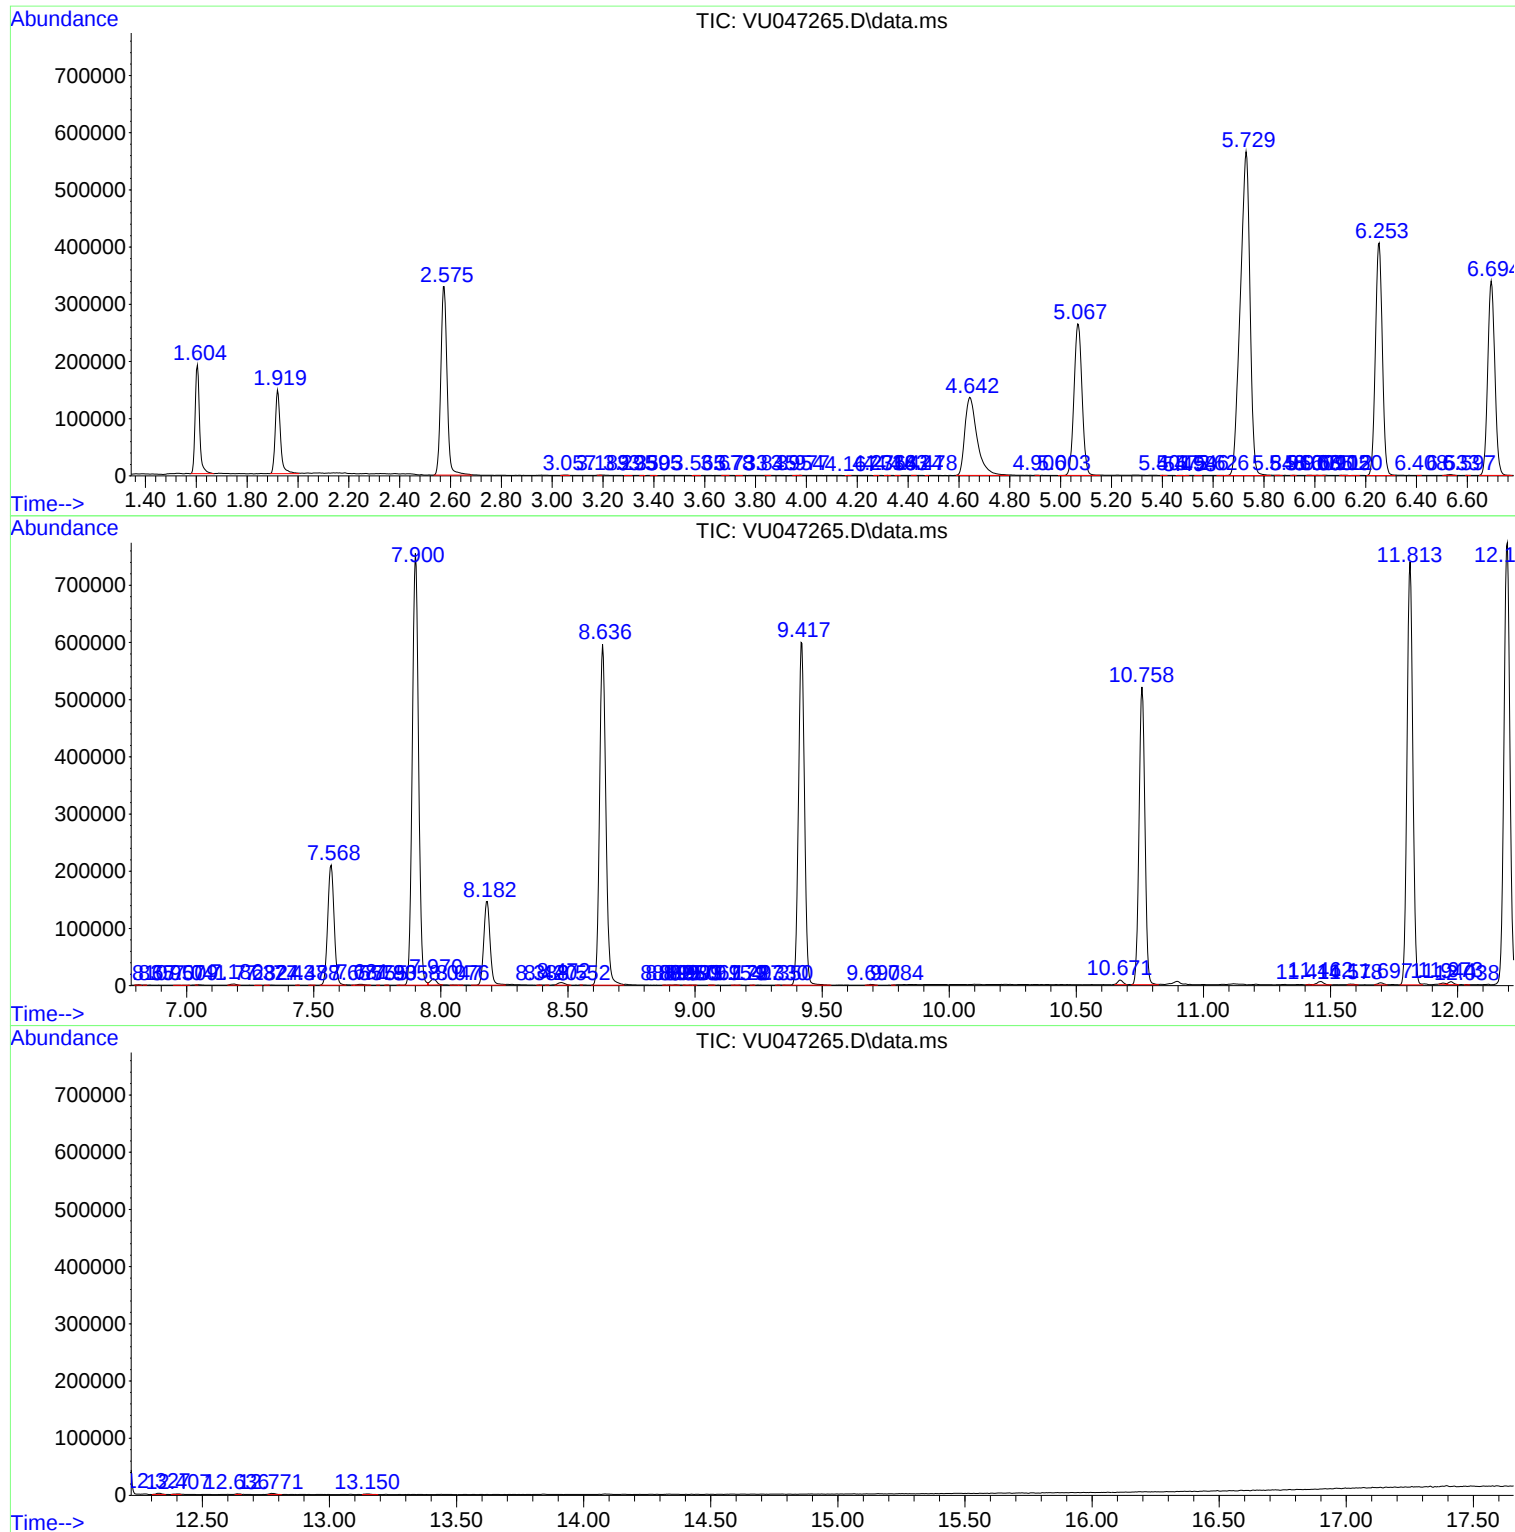

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
Data File : VU047265.D
Acq On : 25 Feb 2022 11:36
Operator : SY/MD
Sample : VU0225WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK071

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
Data File : VU047265.D
Acq On : 25 Feb 2022 11:36
Operator : SY/MD
Sample : VU0225WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK071

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------