

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047267.D
 Acq On : 25 Feb 2022 12:23
 Operator : SY/MD
 Sample : N1667-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBRL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

Signal : TIC: VU047267.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	100	rVB	145155	169758	14.98%	2.101%
2	1.919	172	180	197	rBV	115694	154711	13.65%	1.915%
3	2.575	371	384	405	rBV	252294	420977	37.15%	5.211%
4	2.716	426	428	435	rVB2	334	235	0.02%	0.003%
5	2.774	443	446	450	rBV3	308	198	0.02%	0.002%
6	2.800	450	454	455	rBV2	205	148	0.01%	0.002%
7	2.864	469	474	475	rBV	283	186	0.02%	0.002%
8	3.031	520	526	529	rBV2	181	223	0.02%	0.003%
9	3.050	529	532	536	rVB3	469	380	0.03%	0.005%
10	3.089	541	544	549	rVB3	258	224	0.02%	0.003%
11	3.131	549	557	561	rBV3	242	308	0.03%	0.004%
12	3.198	565	578	588	rBV4	1378	3330	0.29%	0.041%
13	3.259	593	597	603	rVB4	411	362	0.03%	0.004%
14	3.292	603	607	608	rBV	244	164	0.01%	0.002%
15	3.565	687	692	695	rBV2	171	168	0.01%	0.002%
16	3.584	695	698	700	rBV2	221	148	0.01%	0.002%
17	3.645	712	717	720	rVB2	181	153	0.01%	0.002%
18	3.671	723	725	729	rVB3	237	153	0.01%	0.002%
19	3.986	819	823	826	rBV	183	149	0.01%	0.002%
20	4.173	876	881	886	rVB3	168	188	0.02%	0.002%
21	4.205	886	891	894	rBV2	212	247	0.02%	0.003%
22	4.240	899	902	904	rBV2	178	133	0.01%	0.002%
23	4.282	912	915	919	rVB3	187	146	0.01%	0.002%
24	4.468	968	973	976	rBV2	185	155	0.01%	0.002%
25	4.636	1008	1025	1062	rBV	114927	338479	29.87%	4.190%
26	4.915	1108	1112	1114	rBV3	380	244	0.02%	0.003%
27	4.970	1125	1129	1132	rBV2	280	195	0.02%	0.002%
28	5.066	1143	1159	1180	rBV	201112	439407	38.78%	5.439%
29	5.282	1223	1226	1228	rBV3	276	202	0.02%	0.003%
30	5.362	1248	1251	1253	rBV	216	150	0.01%	0.002%
31	5.504	1292	1295	1300	rVB2	176	174	0.02%	0.002%
32	5.558	1308	1312	1315	rBV3	179	154	0.01%	0.002%
33	5.729	1341	1365	1392	rBV2	426845	1133142	100.00%	14.027%
34	5.838	1395	1399	1403	rVV3	359	428	0.04%	0.005%
35	5.861	1403	1406	1413	rVV3	305	425	0.04%	0.005%
36	5.918	1421	1424	1429	rVV3	168	202	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047267.D
 Acq On : 25 Feb 2022 12:23
 Operator : SY/MD
 Sample : N1667-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBRL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	5.967	1434	1439	1441	rVB3	382	241	0.02%	0.003%
38	5.983	1441	1444	1445	rBV2	228	144	0.01%	0.002%
39	6.047	1457	1464	1467	rVB2	393	375	0.03%	0.005%
40	6.086	1474	1476	1481	rVB2	176	167	0.01%	0.002%
41	6.108	1481	1483	1487	rBV3	159	134	0.01%	0.002%
42	6.131	1487	1490	1494	rVB3	170	144	0.01%	0.002%
43	6.250	1512	1527	1549	rVV	163643	306887	27.08%	3.799%
44	6.430	1576	1583	1585	rBV3	180	185	0.02%	0.002%
45	6.472	1591	1596	1599	rBV2	148	142	0.01%	0.002%
46	6.533	1608	1615	1623	rBV4	752	1183	0.10%	0.015%
47	6.693	1649	1665	1685	rBV	257373	496992	43.86%	6.152%
48	6.796	1695	1697	1699	rBV3	396	167	0.01%	0.002%
49	6.809	1699	1701	1704	rBV3	385	255	0.02%	0.003%
50	6.841	1707	1711	1714	rVB3	758	553	0.05%	0.007%
51	6.883	1719	1724	1728	rVV4	208	169	0.01%	0.002%
52	6.928	1735	1738	1743	rBV2	174	150	0.01%	0.002%
53	6.960	1744	1748	1751	rVB2	213	140	0.01%	0.002%
54	7.044	1770	1774	1782	rVB3	534	731	0.06%	0.009%
55	7.185	1805	1818	1822	rBV3	1374	2152	0.19%	0.027%
56	7.246	1835	1837	1845	rVB3	304	342	0.03%	0.004%
57	7.298	1845	1853	1855	rBV2	198	258	0.02%	0.003%
58	7.497	1913	1915	1920	rVB	275	163	0.01%	0.002%
59	7.568	1920	1937	1959	rBV	155380	270381	23.86%	3.347%
60	7.680	1965	1972	1981	rVB3	1073	1811	0.16%	0.022%
61	7.793	2006	2007	2016	rVB4	318	369	0.03%	0.005%
62	7.899	2023	2040	2055	rBV	557472	959395	84.67%	11.876%
63	7.970	2056	2062	2076	rVB	10336	17092	1.51%	0.212%
64	8.076	2092	2095	2099	rVB3	542	379	0.03%	0.005%
65	8.179	2113	2127	2144	rBV	108453	182458	16.10%	2.259%
66	8.475	2206	2219	2232	rBV	18349	33049	2.92%	0.409%
67	8.555	2242	2244	2249	rVB2	305	229	0.02%	0.003%
68	8.635	2256	2269	2293	rBV	428057	729715	64.40%	9.033%
69	8.803	2320	2321	2326	rVB3	303	205	0.02%	0.003%
70	8.870	2335	2342	2345	rBV4	397	466	0.04%	0.006%
71	8.899	2349	2351	2360	rVB3	370	248	0.02%	0.003%
72	8.973	2372	2374	2378	rBV2	222	205	0.02%	0.003%
73	9.188	2437	2441	2448	rVB2	339	402	0.04%	0.005%
74	9.233	2452	2455	2458	rBV2	196	162	0.01%	0.002%
75	9.288	2468	2472	2477	rVB2	214	190	0.02%	0.002%
76	9.417	2500	2512	2531	rBV	237595	385446	34.02%	4.771%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047267.D
 Acq On : 25 Feb 2022 12:23
 Operator : SY/MD
 Sample : N1667-02
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBRL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

77	9.571	2554	2560	2566	rBV4	607	737	0.07%	0.009%
78	9.639	2576	2581	2585	rVB3	329	301	0.03%	0.004%
79	9.664	2585	2589	2591	rBV2	324	254	0.02%	0.003%
80	9.693	2591	2598	2609	rVB2	2770	3910	0.35%	0.048%
81	9.870	2639	2653	2657	rBV4	930	1951	0.17%	0.024%
82	10.671	2895	2902	2909	rVB2	4309	6577	0.58%	0.081%
83	10.758	2916	2929	2946	rBV	374854	596597	52.65%	7.385%
84	10.893	2962	2971	2987	rVB	23383	40633	3.59%	0.503%
85	11.089	3023	3032	3037	rBV6	1672	2703	0.24%	0.033%
86	11.204	3064	3068	3076	rBV5	855	1013	0.09%	0.013%
87	11.426	3135	3137	3138	rBV	332	145	0.01%	0.002%
88	11.462	3138	3148	3159	rVB4	3744	6477	0.57%	0.080%
89	11.577	3179	3184	3185	rBV4	717	656	0.06%	0.008%
90	11.693	3213	3220	3233	rBV5	2311	3524	0.31%	0.044%
91	11.812	3245	3257	3272	rBV	280724	441314	38.95%	5.463%
92	11.944	3292	3298	3301	rBV2	1389	1646	0.15%	0.020%
93	12.063	3332	3335	3339	rBV3	575	395	0.03%	0.005%
94	12.192	3362	3375	3392	rVB	559964	892467	78.76%	11.048%
95	12.323	3411	3416	3427	rBV5	1180	1748	0.15%	0.022%
96	12.635	3511	3513	3521	rVB4	958	1079	0.10%	0.013%
97	12.774	3547	3556	3567	rVB2	6643	10473	0.92%	0.130%
98	12.828	3567	3573	3576	rBV3	1311	1243	0.11%	0.015%
99	13.028	3633	3635	3638	rBV4	387	219	0.02%	0.003%
100	14.089	3957	3965	3971	rBV	1410	2207	0.19%	0.027%




Sum of corrected areas: 8078191

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
Data File : VU047267.D
Acq On : 25 Feb 2022 12:23
Operator : SY/MD
Sample : N1667-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBRL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

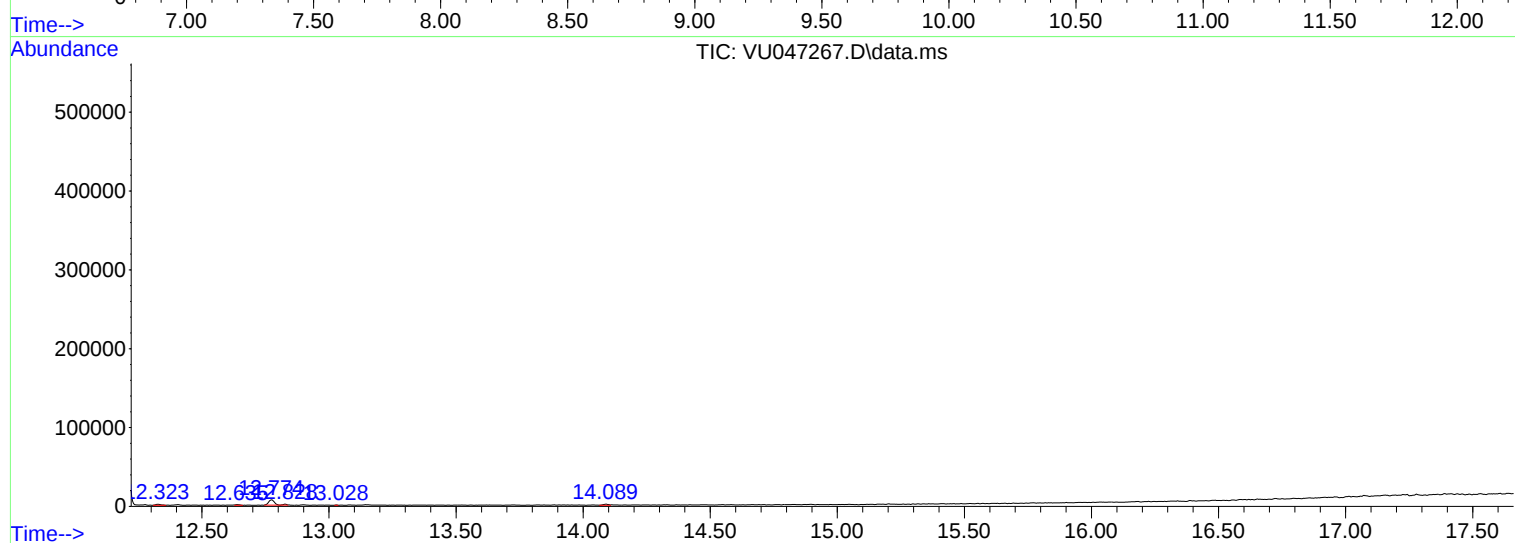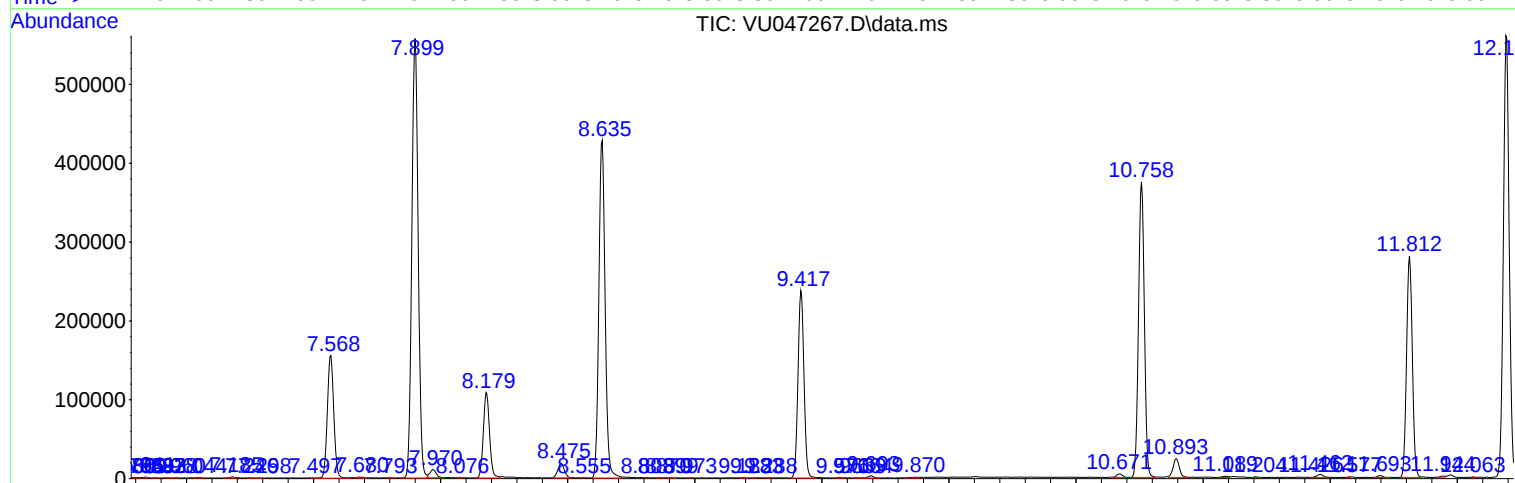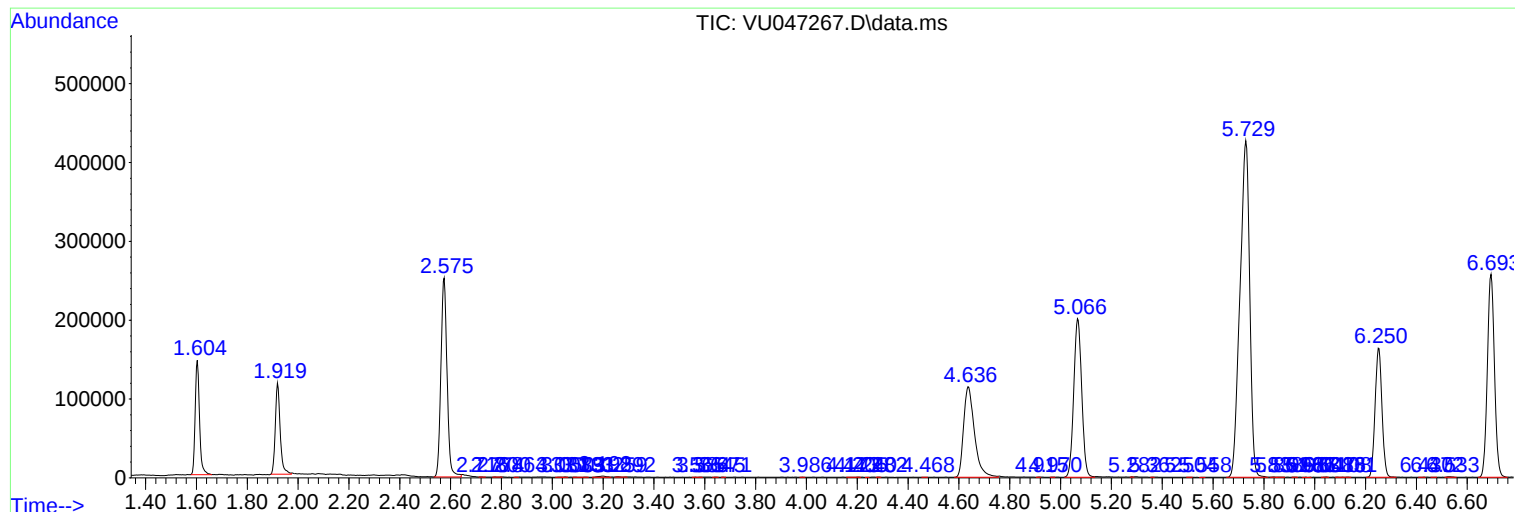

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
Data File : VU047267.D
Acq On : 25 Feb 2022 12:23
Operator : SY/MD
Sample : N1667-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBRL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
Data File : VU047267.D
Acq On : 25 Feb 2022 12:23
Operator : SY/MD
Sample : N1667-02
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBRL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------