

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047268.D
 Acq On : 25 Feb 2022 12:55
 Operator : SY/MD
 Sample : N1667-02RE
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBRL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

Signal : TIC: VU047268.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	100	rVB	198080	234869	15.11%	1.789%
2	1.919	171	180	195	rBV	156771	212225	13.65%	1.617%
3	2.572	371	383	417	rBV	345180	587613	37.81%	4.477%
4	2.774	444	446	449	rVB4	210	126	0.01%	0.001%
5	2.800	449	454	457	rBV	321	293	0.02%	0.002%
6	2.954	494	502	505	rBV3	459	589	0.04%	0.004%
7	2.974	505	508	513	rVB2	431	341	0.02%	0.003%
8	3.006	517	518	523	rVB2	211	131	0.01%	0.001%
9	3.051	527	532	535	rBV3	516	554	0.04%	0.004%
10	3.118	549	553	556	rVB2	205	154	0.01%	0.001%
11	3.150	556	563	565	rBV2	182	203	0.01%	0.002%
12	3.195	567	577	590	rVB2	1644	3404	0.22%	0.026%
13	3.279	600	603	605	rBV2	241	144	0.01%	0.001%
14	3.356	625	627	631	rVB2	248	163	0.01%	0.001%
15	3.388	631	637	642	rBV3	209	291	0.02%	0.002%
16	3.411	642	644	648	rVB	256	177	0.01%	0.001%
17	3.446	652	655	658	rBV2	202	155	0.01%	0.001%
18	3.466	658	661	668	rBV	240	212	0.01%	0.002%
19	3.745	745	748	751	rBV2	219	173	0.01%	0.001%
20	3.768	753	755	760	rVV3	190	160	0.01%	0.001%
21	3.858	779	783	787	rVV2	236	213	0.01%	0.002%
22	3.900	792	796	801	rVV2	202	183	0.01%	0.001%
23	3.983	816	822	826	rBV2	153	190	0.01%	0.001%
24	4.044	836	841	845	rBV2	186	193	0.01%	0.001%
25	4.163	874	878	882	rVB3	158	154	0.01%	0.001%
26	4.234	896	900	903	rVV2	165	153	0.01%	0.001%
27	4.250	903	905	909	rVB	185	127	0.01%	0.001%
28	4.279	909	914	917	rBV2	235	232	0.01%	0.002%
29	4.314	921	925	929	rVB3	271	251	0.02%	0.002%
30	4.340	929	933	938	rBV2	284	252	0.02%	0.002%
31	4.453	964	968	971	rBV3	176	145	0.01%	0.001%
32	4.510	981	986	989	rVB3	193	187	0.01%	0.001%
33	4.556	996	1000	1007	rVB2	239	237	0.02%	0.002%
34	4.639	1008	1026	1071	rBV	148745	452838	29.14%	3.450%
35	4.945	1118	1121	1125	rVB	229	151	0.01%	0.001%
36	5.067	1139	1159	1187	rBV	280028	612817	39.43%	4.669%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047268.D
 Acq On : 25 Feb 2022 12:55
 Operator : SY/MD
 Sample : N1667-02RE
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBRL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	5.289	1223	1228	1237	rVB4	577	892	0.06%	0.007%
38	5.359	1245	1250	1254	rBV3	165	185	0.01%	0.001%
39	5.385	1257	1258	1265	rVB3	300	194	0.01%	0.001%
40	5.430	1269	1272	1274	rBV2	204	140	0.01%	0.001%
41	5.498	1290	1293	1297	rVB2	251	152	0.01%	0.001%
42	5.581	1314	1319	1322	rBV3	145	135	0.01%	0.001%
43	5.655	1337	1342	1343	rBV3	164	134	0.01%	0.001%
44	5.729	1343	1365	1396	rBV2	588382	1554207	100.00%	11.841%
45	5.864	1404	1407	1410	rBV2	137	130	0.01%	0.001%
46	5.967	1436	1439	1444	rVB2	676	612	0.04%	0.005%
47	5.990	1444	1446	1449	rVB2	425	229	0.01%	0.002%
48	6.012	1449	1453	1456	rBV	252	189	0.01%	0.001%
49	6.031	1456	1459	1472	rBV4	365	643	0.04%	0.005%
50	6.253	1512	1528	1548	rBV	499055	929698	59.82%	7.083%
51	6.427	1578	1582	1589	rVB2	262	320	0.02%	0.002%
52	6.456	1589	1591	1595	rBV3	239	133	0.01%	0.001%
53	6.530	1607	1614	1625	rBV5	1146	2091	0.13%	0.016%
54	6.629	1641	1645	1650	rBV3	168	183	0.01%	0.001%
55	6.694	1650	1665	1685	rBV	358056	691006	44.46%	5.265%
56	6.774	1688	1690	1694	rVB3	199	130	0.01%	0.001%
57	6.803	1694	1699	1700	rBV2	397	346	0.02%	0.003%
58	6.835	1705	1709	1710	rBV3	525	331	0.02%	0.003%
59	6.880	1720	1723	1728	rVB	317	225	0.01%	0.002%
60	6.912	1728	1733	1737	rBV2	226	224	0.01%	0.002%
61	7.044	1766	1774	1782	rBV4	911	1611	0.10%	0.012%
62	7.182	1808	1817	1827	rBV2	2139	3347	0.22%	0.026%
63	7.327	1858	1862	1866	rVB2	211	136	0.01%	0.001%
64	7.353	1866	1870	1875	rBV2	197	194	0.01%	0.001%
65	7.379	1875	1878	1885	rVB3	205	229	0.01%	0.002%
66	7.481	1908	1910	1915	rVV	294	206	0.01%	0.002%
67	7.568	1924	1937	1954	rBV	220738	377075	24.26%	2.873%
68	7.684	1968	1973	1985	rVB5	1501	2391	0.15%	0.018%
69	7.800	2005	2009	2012	rBV2	327	344	0.02%	0.003%
70	7.899	2025	2040	2055	rBV	794470	1345964	86.60%	10.255%
71	7.973	2056	2063	2077	rVB	13465	22361	1.44%	0.170%
72	8.182	2115	2128	2149	rBV	150540	256250	16.49%	1.952%
73	8.324	2170	2172	2181	rVB3	523	505	0.03%	0.004%
74	8.475	2207	2219	2234	rBV2	15876	29435	1.89%	0.224%
75	8.552	2241	2243	2246	rVB2	484	300	0.02%	0.002%
76	8.571	2246	2249	2252	rBV	203	139	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047268.D
 Acq On : 25 Feb 2022 12:55
 Operator : SY/MD
 Sample : N1667-02RE
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBRL2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

77	8.636	2255	2269	2298	rBV	596437	1006329	64.75%	7.667%
78	8.790	2315	2317	2320	rVV2	341	164	0.01%	0.001%
79	8.816	2323	2325	2328	rVB2	390	204	0.01%	0.002%
80	8.928	2355	2360	2363	rBV2	331	250	0.02%	0.002%
81	9.182	2435	2439	2442	rVB3	216	150	0.01%	0.001%
82	9.263	2455	2464	2467	rBV2	375	432	0.03%	0.003%
83	9.420	2496	2513	2543	rBV	707754	1169871	75.27%	8.913%
84	9.571	2553	2560	2567	rBV2	912	1495	0.10%	0.011%
85	9.697	2590	2599	2607	rBV2	3364	5774	0.37%	0.044%
86	10.674	2895	2903	2912	rVB2	7301	11316	0.73%	0.086%
87	10.758	2917	2929	2949	rBV	534300	851561	54.79%	6.488%
88	10.896	2961	2972	2991	rVB	21537	39145	2.52%	0.298%
89	11.205	3064	3068	3077	rVB5	1383	1494	0.10%	0.011%
90	11.243	3077	3080	3086	rBV4	389	429	0.03%	0.003%
91	11.417	3131	3134	3135	rBV2	459	284	0.02%	0.002%
92	11.462	3139	3148	3162	rVB2	6180	10505	0.68%	0.080%
93	11.581	3178	3185	3192	rBV3	1521	2109	0.14%	0.016%
94	11.697	3213	3221	3231	rVB3	3515	5523	0.36%	0.042%
95	11.812	3244	3257	3274	rBV	889581	1376345	88.56%	10.486%
96	11.947	3289	3299	3302	rBV6	2378	4115	0.26%	0.031%
97	12.195	3360	3376	3395	rBV	809896	1292840	83.18%	9.850%
98	12.639	3510	3514	3532	rVB7	1211	2280	0.15%	0.017%
99	12.774	3548	3556	3568	rBV2	5865	9060	0.58%	0.069%
100	14.938	4227	4229	4231	rBV2	810	408	0.03%	0.003%




Sum of corrected areas: 13125399

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
Data File : VU047268.D
Acq On : 25 Feb 2022 12:55
Operator : SY/MD
Sample : N1667-02RE
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBRL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

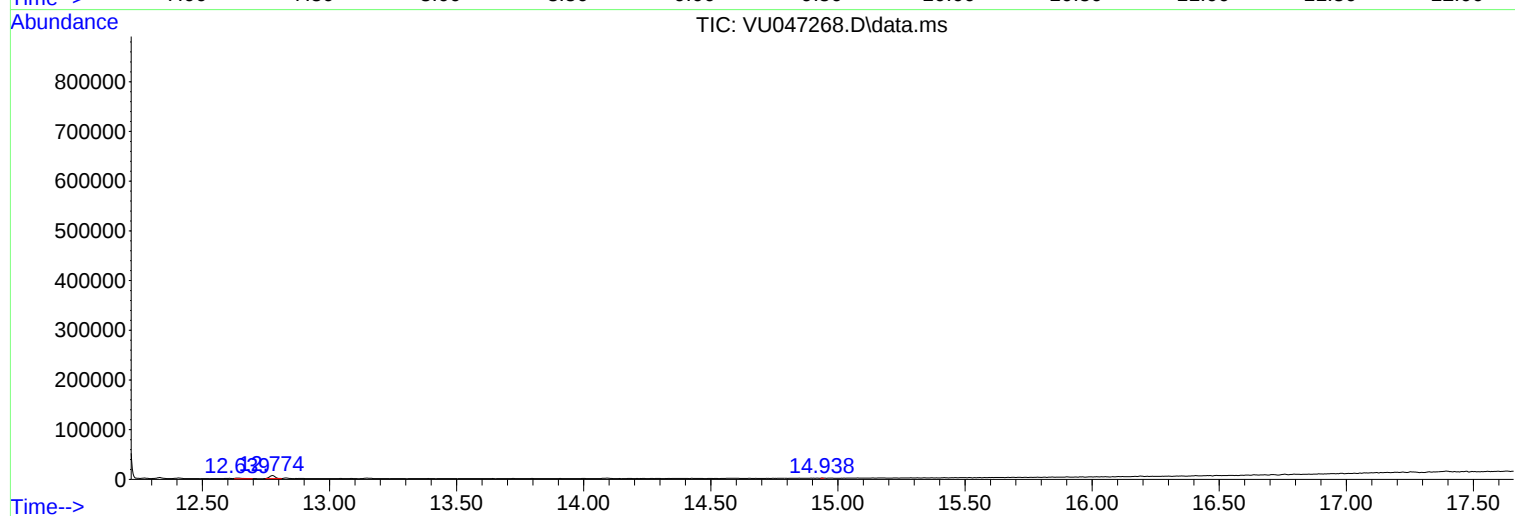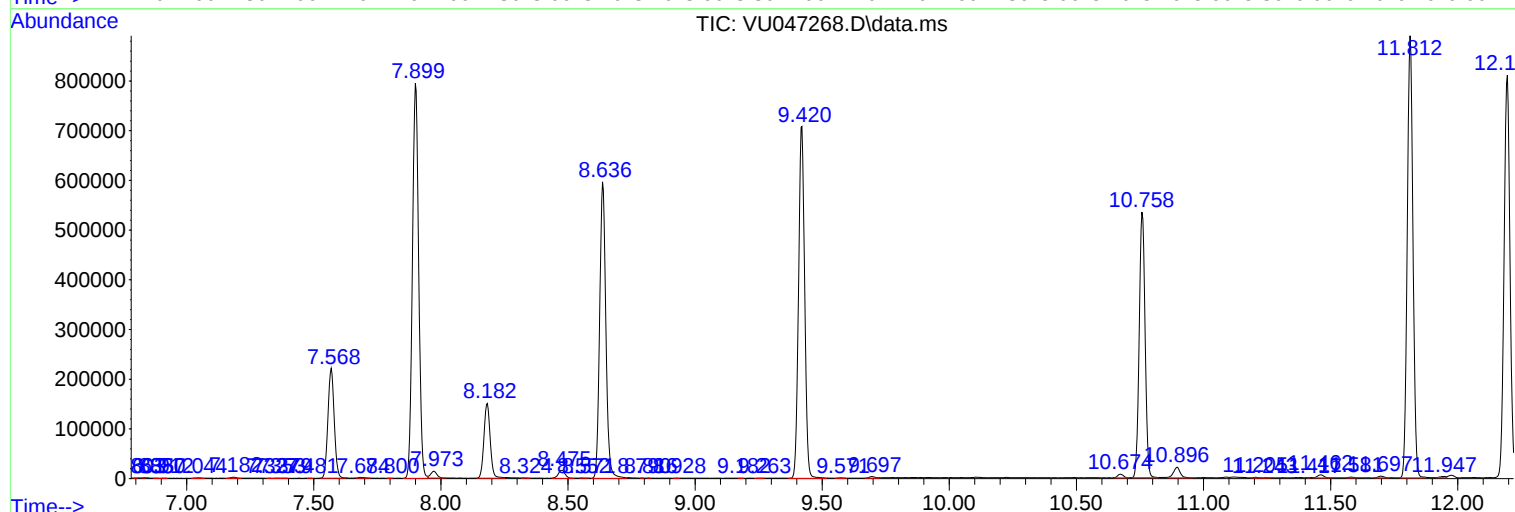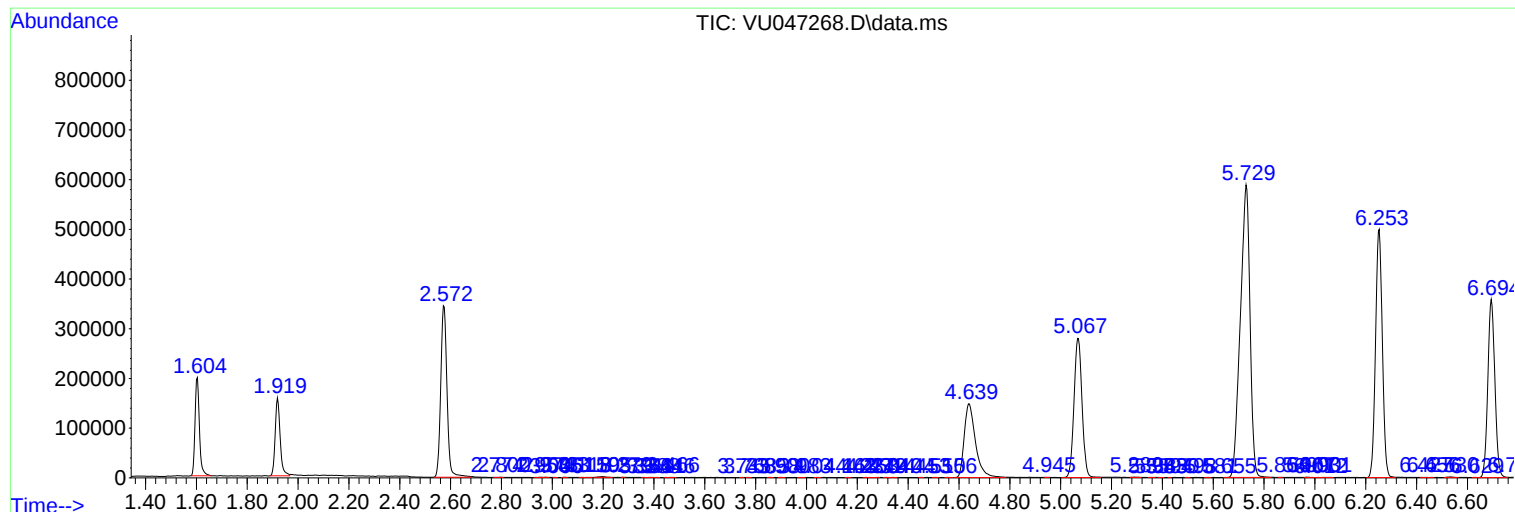

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
Data File : VU047268.D
Acq On : 25 Feb 2022 12:55
Operator : SY/MD
Sample : N1667-02RE
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBRL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
Data File : VU047268.D
Acq On : 25 Feb 2022 12:55
Operator : SY/MD
Sample : N1667-02RE
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBRL2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------