

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047271.D
 Acq On : 25 Feb 2022 15:16
 Operator : SY/MD
 Sample : N1667-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBRL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

Signal : TIC: VU047271.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.604	74	82	98	rBV	182208	217096	14.77%	1.798%
2	1.919	171	180	202	rBV	144217	198983	13.54%	1.648%
3	2.475	350	353	357	rVB4	721	605	0.04%	0.005%
4	2.501	357	361	363	rBV3	244	196	0.01%	0.002%
5	2.571	371	383	405	rBV	324147	543655	36.99%	4.502%
6	2.790	448	451	452	rBV3	279	173	0.01%	0.001%
7	2.829	459	463	465	rBV2	234	176	0.01%	0.001%
8	2.896	480	484	490	rVV3	224	203	0.01%	0.002%
9	2.938	494	497	499	rBV3	248	186	0.01%	0.002%
10	3.044	527	530	533	rBV3	740	659	0.04%	0.005%
11	3.083	539	542	545	rBV2	240	153	0.01%	0.001%
12	3.192	566	576	579	rBV	1149	1957	0.13%	0.016%
13	3.243	589	592	597	rVB3	156	163	0.01%	0.001%
14	3.314	611	614	618	rBV2	265	189	0.01%	0.002%
15	3.401	638	641	644	rVB	254	142	0.01%	0.001%
16	3.417	644	646	654	rVB3	167	173	0.01%	0.001%
17	3.465	654	661	665	rBV3	136	142	0.01%	0.001%
18	3.504	665	673	676	rBV2	180	229	0.02%	0.002%
19	3.620	704	709	712	rVB2	165	141	0.01%	0.001%
20	3.687	726	730	734	rVV2	173	162	0.01%	0.001%
21	3.726	738	742	749	rVB2	231	257	0.02%	0.002%
22	4.076	844	851	853	rVV3	151	144	0.01%	0.001%
23	4.356	932	938	940	rBV3	207	193	0.01%	0.002%
24	4.449	962	967	970	rBV	191	150	0.01%	0.001%
25	4.465	970	972	978	rVB2	143	133	0.01%	0.001%
26	4.494	978	981	984	rBV2	221	143	0.01%	0.001%
27	4.571	1001	1005	1007	rBV2	193	147	0.01%	0.001%
28	4.639	1008	1026	1063	rBV	140583	429883	29.25%	3.560%
29	4.909	1108	1110	1116	rVB2	188	157	0.01%	0.001%
30	4.941	1116	1120	1122	rBV2	162	148	0.01%	0.001%
31	5.067	1143	1159	1180	rBV	261501	569780	38.76%	4.718%
32	5.192	1195	1198	1199	rBV3	280	149	0.01%	0.001%
33	5.295	1222	1230	1233	rBV4	395	587	0.04%	0.005%
34	5.369	1250	1253	1256	rBV2	308	216	0.01%	0.002%
35	5.411	1262	1266	1274	rVB3	139	173	0.01%	0.001%
36	5.494	1288	1292	1296	rVV	125	142	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047271.D
 Acq On : 25 Feb 2022 15:16
 Operator : SY/MD
 Sample : N1667-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBRL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

37	5.533	1300	1304	1310	rVB3	141	154	0.01%	0.001%
38	5.604	1323	1326	1329	rVB3	187	129	0.01%	0.001%
39	5.632	1329	1335	1338	rBV2	237	262	0.02%	0.002%
40	5.729	1342	1365	1386	rBV2	556501	1469873	100.00%	12.172%
41	5.970	1436	1440	1448	rVV4	600	708	0.05%	0.006%
42	6.025	1453	1457	1460	rVV	215	230	0.02%	0.002%
43	6.050	1460	1465	1473	rVB4	471	672	0.05%	0.006%
44	6.118	1481	1486	1488	rBV	469	389	0.03%	0.003%
45	6.253	1512	1528	1552	rVV	433053	818979	55.72%	6.782%
46	6.375	1563	1566	1569	rBV3	248	148	0.01%	0.001%
47	6.407	1574	1576	1580	rVB2	334	211	0.01%	0.002%
48	6.530	1607	1614	1622	rVB2	1156	1653	0.11%	0.014%
49	6.594	1631	1634	1636	rVV3	366	227	0.02%	0.002%
50	6.613	1636	1640	1644	rVB3	238	191	0.01%	0.002%
51	6.694	1650	1665	1685	rBV	340095	650922	44.28%	5.390%
52	6.796	1694	1697	1698	rBV	303	178	0.01%	0.001%
53	6.870	1717	1720	1725	rBV3	282	215	0.01%	0.002%
54	7.044	1767	1774	1782	rVV3	1013	1586	0.11%	0.013%
55	7.185	1806	1818	1826	rVB2	2065	3359	0.23%	0.028%
56	7.230	1829	1832	1834	rBV2	207	170	0.01%	0.001%
57	7.282	1843	1848	1851	rVB2	320	259	0.02%	0.002%
58	7.356	1867	1871	1874	rBV3	325	214	0.01%	0.002%
59	7.372	1874	1876	1880	rBV2	258	212	0.01%	0.002%
60	7.568	1921	1937	1959	rBV	205257	357759	24.34%	2.962%
61	7.648	1959	1962	1967	rVB4	487	365	0.02%	0.003%
62	7.690	1967	1975	1981	rBV3	1131	1946	0.13%	0.016%
63	7.784	2001	2004	2006	rBV2	268	215	0.01%	0.002%
64	7.899	2025	2040	2055	rBV	734032	1258948	85.65%	10.425%
65	7.970	2057	2062	2079	rVB	10948	18089	1.23%	0.150%
66	8.054	2085	2088	2089	rBV2	250	164	0.01%	0.001%
67	8.111	2103	2106	2110	rBV2	290	207	0.01%	0.002%
68	8.182	2115	2128	2148	rBV	142568	240989	16.40%	1.996%
69	8.391	2190	2193	2197	rBV3	249	196	0.01%	0.002%
70	8.414	2197	2200	2203	rVB3	358	187	0.01%	0.002%
71	8.475	2209	2219	2229	rVV2	10023	17947	1.22%	0.149%
72	8.517	2229	2232	2236	rVB3	375	280	0.02%	0.002%
73	8.636	2255	2269	2294	rBV	555734	946892	64.42%	7.841%
74	8.787	2309	2316	2328	rVB6	3311	5219	0.36%	0.043%
75	8.912	2351	2355	2358	rVV3	198	155	0.01%	0.001%
76	9.021	2386	2389	2393	rVB2	211	142	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047271.D
 Acq On : 25 Feb 2022 15:16
 Operator : SY/MD
 Sample : N1667-01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBRL0

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis

77	9.047	2393	2397	2399	rBV2	218	150	0.01%	0.001%
78	9.118	2416	2419	2425	rBV2	296	213	0.01%	0.002%
79	9.237	2450	2456	2458	rBV2	241	195	0.01%	0.002%
80	9.301	2470	2476	2479	rBV4	289	281	0.02%	0.002%
81	9.353	2488	2492	2494	rBV2	205	143	0.01%	0.001%
82	9.420	2499	2513	2543	rBV	625090	1032828	70.27%	8.553%
83	9.542	2548	2551	2555	rVB	317	176	0.01%	0.001%
84	9.574	2555	2561	2565	rBV	480	512	0.03%	0.004%
85	9.693	2591	2598	2608	rVB5	1361	2370	0.16%	0.020%
86	9.774	2612	2623	2631	rBV4	949	2132	0.15%	0.018%
87	10.674	2895	2903	2916	rVB2	5950	8920	0.61%	0.074%
88	10.758	2916	2929	2947	rBV	502249	792514	53.92%	6.563%
89	10.893	2961	2971	2987	rVB2	20478	38861	2.64%	0.322%
90	11.459	3139	3147	3158	rVB5	5562	10020	0.68%	0.083%
91	11.697	3212	3221	3233	rBV3	3387	5907	0.40%	0.049%
92	11.748	3233	3237	3241	rVB2	662	483	0.03%	0.004%
93	11.812	3244	3257	3273	rBV	766434	1198866	81.56%	9.927%
94	12.195	3360	3376	3393	rVB	740351	1196169	81.38%	9.905%
95	12.327	3412	3417	3427	rBV6	2289	3617	0.25%	0.030%
96	12.516	3474	3476	3478	rBV	342	175	0.01%	0.001%
97	12.594	3498	3500	3506	rVB3	537	347	0.02%	0.003%
98	12.774	3548	3556	3565	rVB2	6079	9661	0.66%	0.080%
99	13.147	3662	3672	3682	rBV6	1369	3019	0.21%	0.025%
100	14.716	4158	4160	4163	rBV3	434	269	0.02%	0.002%


Sum of corrected areas: 12076254

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
Data File : VU047271.D
Acq On : 25 Feb 2022 15:16
Operator : SY/MD
Sample : N1667-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBRL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

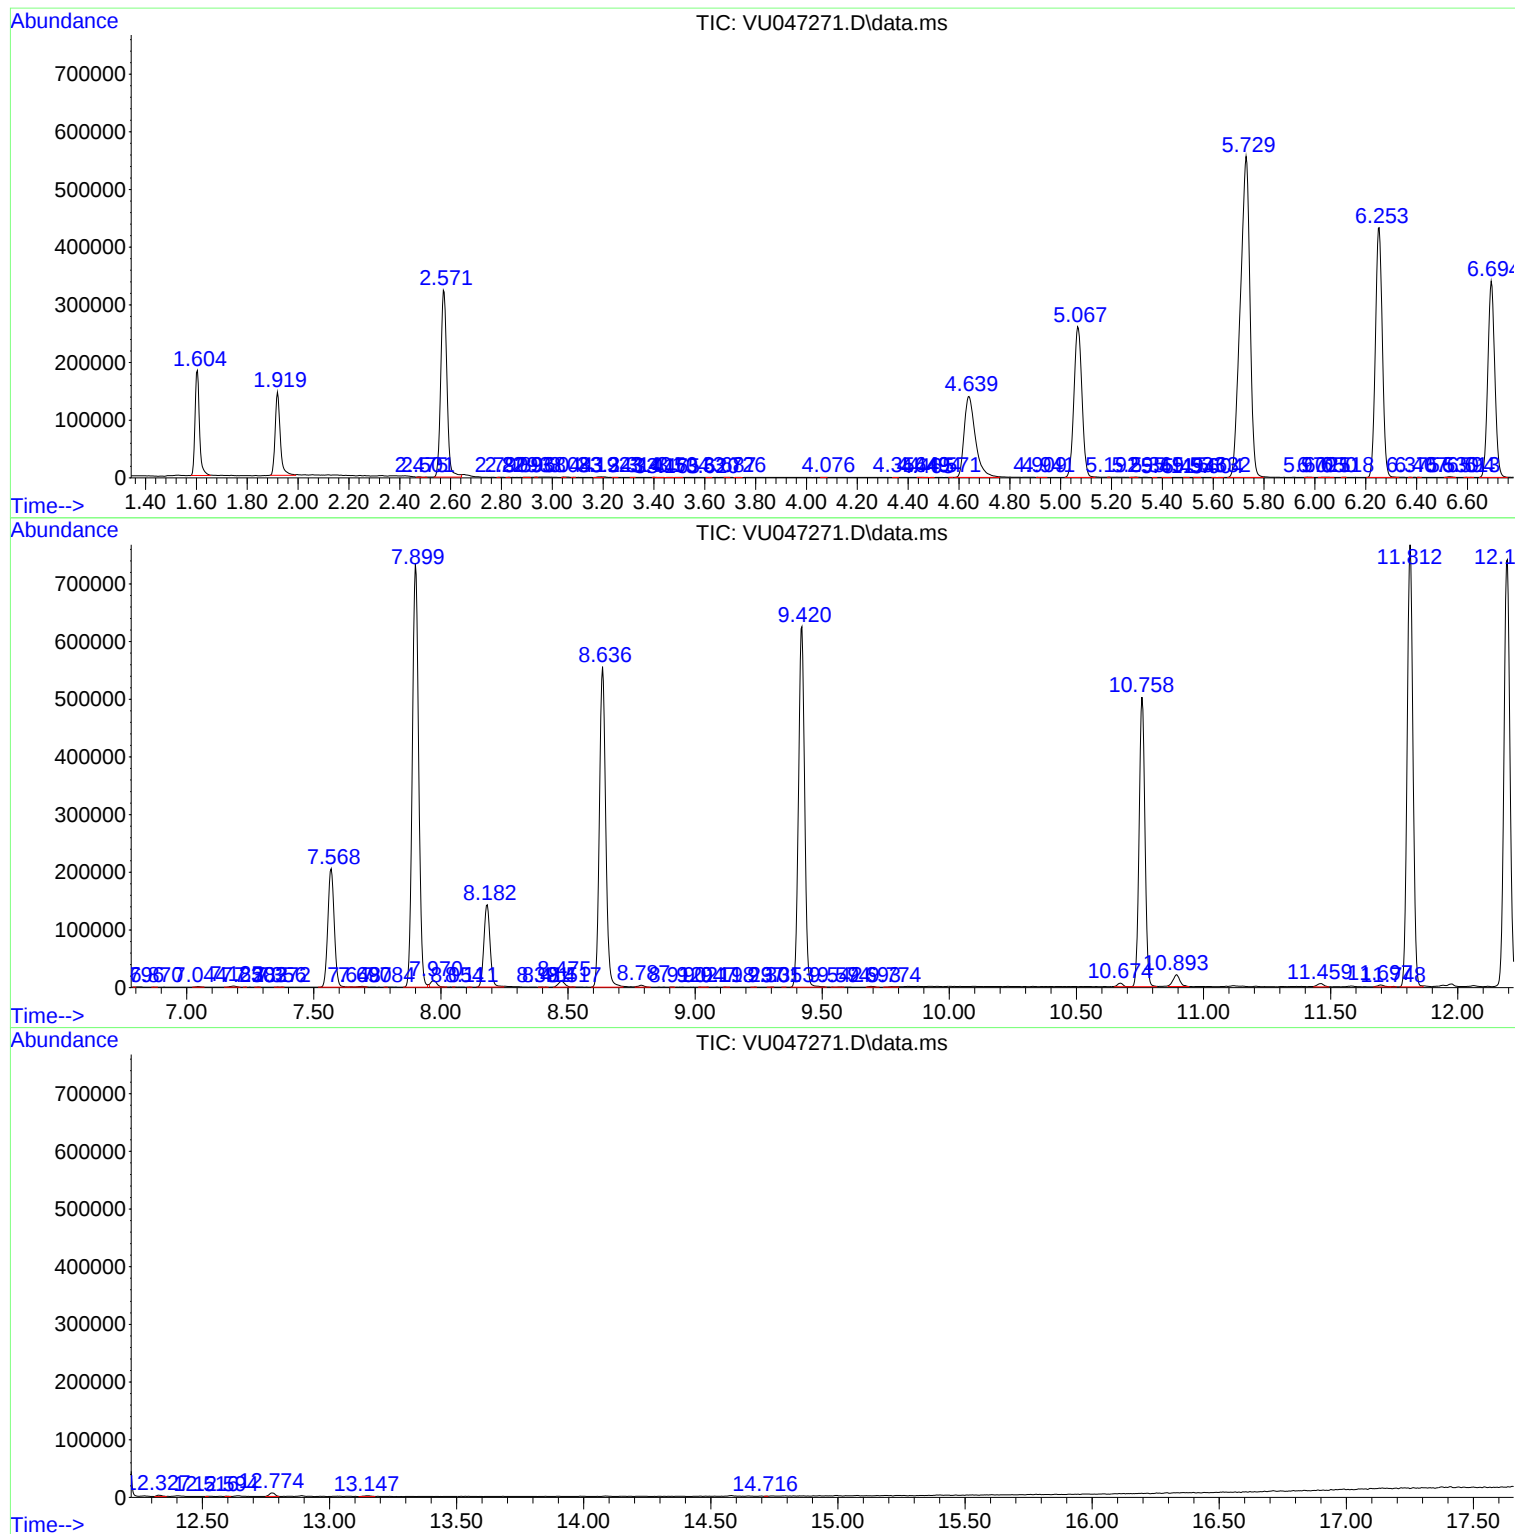

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
Data File : VU047271.D
Acq On : 25 Feb 2022 15:16
Operator : SY/MD
Sample : N1667-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBRL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
Data File : VU047271.D
Acq On : 25 Feb 2022 15:16
Operator : SY/MD
Sample : N1667-01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBRL0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------