


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022522\
 Data File : VU047262.D
 Acq On : 25 Feb 2022 09:01
 Operator : SY/MD
 Sample : BFB047
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB047

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021022WMA.M
 Title : VOC Analysis
 Last Update : Mon Feb 28 02:01:00 2022

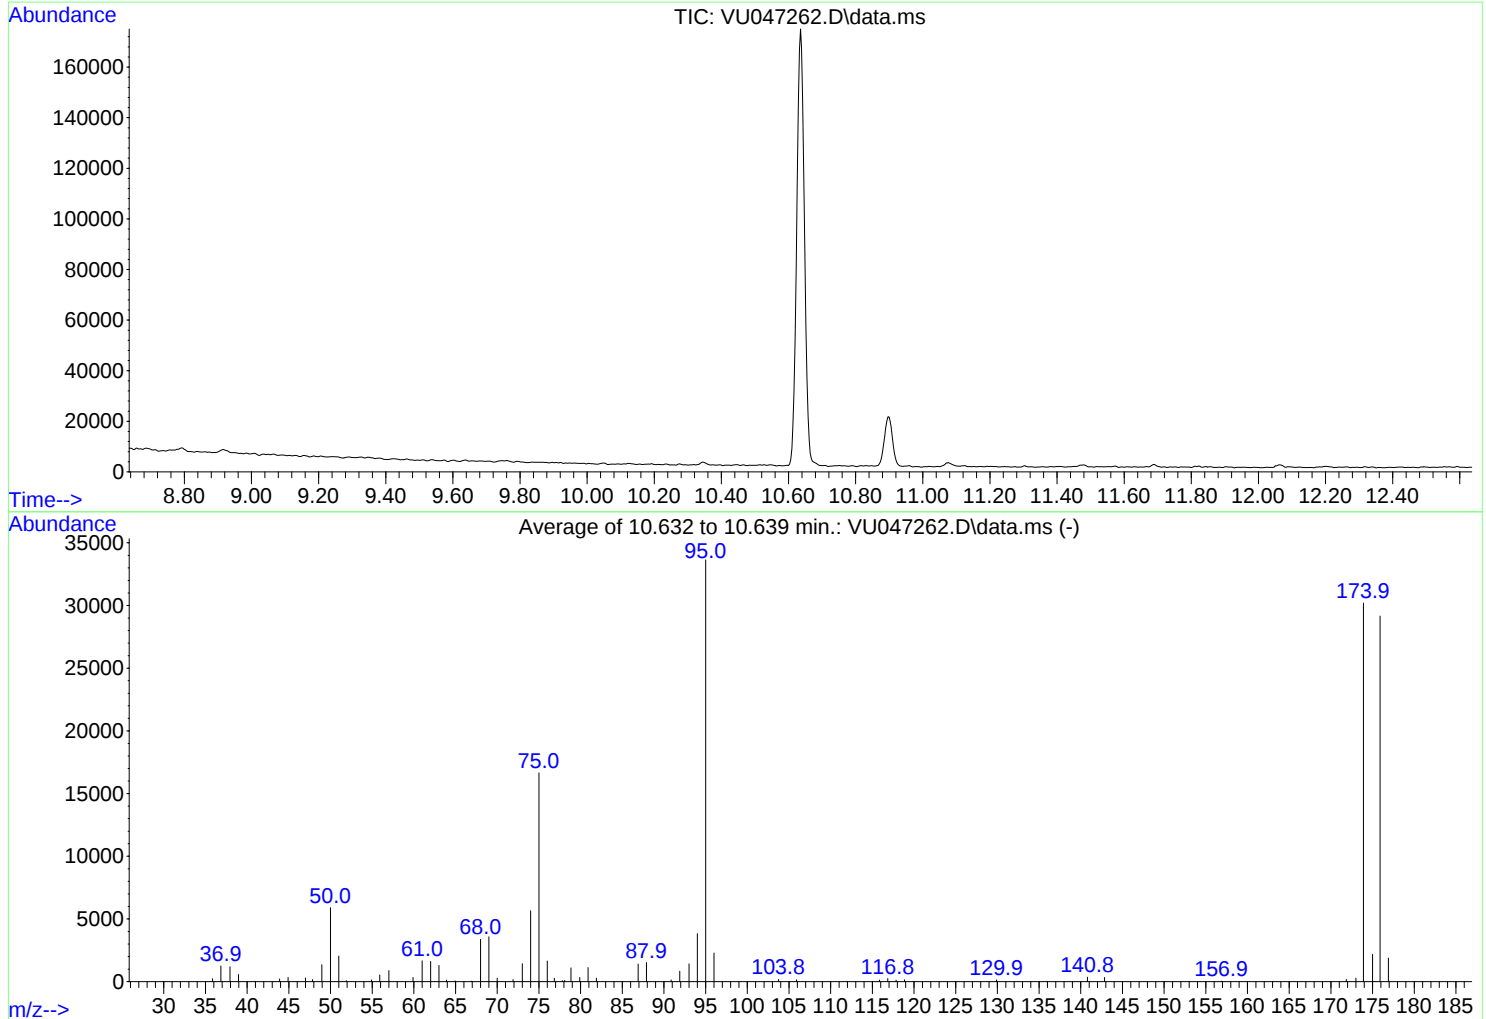

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2878

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.5	5890	PASS
75	95	30	80	49.5	16661	PASS
95	95	100	100	100.0	33643	PASS
96	95	5	9	6.8	2283	PASS
173	174	0.00	2	0.9	283	PASS
174	95	50	120	89.8	30200	PASS
175	174	5	9	7.2	2185	PASS
176	174	95	101	96.5	29157	PASS
177	176	5	9	6.4	1874	PASS

m/z	Abundance
35.90	1267.0
36.80	132.0
37.90	448.0
39.90	266.0
43.90	303.0
207.10	162.0

Instrument :
MSVOA_U
ClientSampleId :
BFB047

m/z	Abundance
35.90	1523.0
36.90	1475.0
38.00	1612.0
39.00	587.0
39.90	205.0
43.90	539.0
44.90	310.0
47.10	331.0
47.80	141.0
48.90	1376.0
50.00	5874.0
51.00	2081.0
51.90	119.0
54.90	146.0
55.90	496.0
57.00	869.0
59.90	313.0
61.00	1629.0
62.00	1638.0
63.00	1317.0
63.90	111.0
65.00	106.0
68.00	3435.0
69.00	3587.0
70.00	284.0
71.90	159.0
73.00	1472.0
74.00	5733.0
75.00	16584.0
76.00	1615.0
76.80	250.0
77.90	128.0
78.90	1133.0
79.90	316.0
80.90	1076.0
81.90	272.0
86.90	1435.0
87.90	1478.0
90.90	154.0
91.90	781.0
93.00	1509.0
94.00	3797.0
95.00	33200.0
96.00	2268.0
103.80	184.0
105.90	168.0
115.90	122.0
116.90	211.0
117.80	111.0
118.90	154.0
129.90	137.0
140.80	359.0
142.90	335.0
171.80	167.0
172.90	274.0
173.90	29056.0
175.00	2150.0
175.90	27840.0
176.90	1819.0
206.90	154.0

Instrument :
MSVOA_U
ClientSampleId :
BFB047

m/z	Abundance
35.90	1518.0
36.90	1402.0
38.00	1693.0
39.00	567.0
39.90	225.0
44.00	528.0
44.90	369.0
47.00	320.0
47.90	167.0
48.90	1406.0
50.00	6052.0
51.00	2105.0
51.90	109.0
54.90	149.0
55.90	563.0
57.00	907.0
59.90	348.0
61.00	1729.0
62.00	1660.0
63.00	1336.0
63.90	119.0
64.90	102.0
68.00	3458.0
69.00	3703.0
70.00	290.0
71.90	178.0
73.00	1460.0
74.00	5812.0
75.00	17208.0
76.00	1705.0
76.90	294.0
78.10	142.0
78.90	1134.0
79.90	342.0
80.90	1142.0
81.90	295.0
86.90	1446.0
87.90	1580.0
90.90	141.0
91.90	841.0
93.00	1459.0
94.00	3953.0
95.00	34552.0
96.00	2369.0
103.70	195.0
105.90	162.0
115.90	138.0
116.80	263.0
117.90	141.0
118.90	172.0
129.90	143.0
140.80	364.0
142.90	338.0
156.90	108.0
171.80	180.0
173.00	281.0
173.90	31208.0
175.00	2240.0
175.90	30152.0
176.90	1923.0
206.90	145.0

Instrument :
MSVOA_U
ClientSampleId :
BFB047

m/z	Abundance
35.90	1458.0
36.90	1283.0
38.00	1619.0
38.90	544.0
39.90	286.0
44.00	483.0
44.90	364.0
46.90	244.0
47.90	184.0
49.00	1266.0
50.00	5744.0
51.00	1937.0
54.90	132.0
55.90	557.0
57.00	876.0
59.90	339.0
61.00	1624.0
62.00	1546.0
63.00	1208.0
63.90	135.0
66.90	105.0
68.00	3223.0
69.00	3443.0
70.00	276.0
71.90	182.0
73.00	1369.0
74.00	5439.0
75.00	16192.0
76.00	1610.0
76.90	271.0
77.70	115.0
78.10	155.0
78.80	1048.0
79.90	324.0
80.90	1138.0
81.90	273.0
86.90	1322.0
87.90	1494.0
90.80	127.0
91.90	880.0
93.00	1280.0
94.00	3746.0
95.00	33176.0
96.00	2213.0
103.80	161.0
105.90	132.0
115.80	128.0
116.80	273.0
117.80	136.0
118.80	148.0
129.90	150.0
140.80	337.0
142.80	334.0
171.90	182.0
173.10	294.0
173.90	30336.0
175.00	2166.0
175.90	29480.0
176.90	1880.0
206.90	143.0

Instrument :
MSVOA_U
ClientSampleId :
BFB047