

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022724\
 Data File : VU057951.D
 Acq On : 27 Feb 2024 13:04
 Operator : MD/SY
 Sample : VU0227WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK046

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

Signal : TIC: VU057951.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.592	86	94	110	rBV	147502	169102	15.97%	2.143%
2	1.904	183	191	209	rVB	116027	150148	14.18%	1.903%
3	2.560	382	395	414	rBV	221850	368123	34.76%	4.665%
4	2.673	428	430	433	rVB3	467	194	0.02%	0.002%
5	2.782	459	464	473	rVB4	802	1356	0.13%	0.017%
6	2.849	483	485	489	rBV2	206	174	0.02%	0.002%
7	2.930	506	510	515	rBV3	227	175	0.02%	0.002%
8	3.039	534	544	556	rVB4	2019	3335	0.31%	0.042%
9	3.322	629	632	636	rBV	246	206	0.02%	0.003%
10	3.637	724	730	734	rBV2	227	238	0.02%	0.003%
11	3.753	763	766	770	rBV2	210	207	0.02%	0.003%
12	3.775	770	773	778	rVV	242	195	0.02%	0.002%
13	3.885	804	807	811	rVB2	239	179	0.02%	0.002%
14	3.917	811	817	821	rBV2	191	252	0.02%	0.003%
15	4.171	890	896	899	rBV2	164	158	0.01%	0.002%
16	4.206	899	907	913	rBV2	308	468	0.04%	0.006%
17	4.306	935	938	943	rVV2	193	160	0.02%	0.002%
18	4.525	997	1006	1012	rBV2	341	465	0.04%	0.006%
19	4.611	1023	1033	1063	rBV	60957	162504	15.35%	2.059%
20	5.052	1154	1170	1197	rBV	186606	410073	38.72%	5.196%
21	5.280	1239	1241	1245	rVB2	382	232	0.02%	0.003%
22	5.319	1249	1253	1257	rBV3	227	227	0.02%	0.003%
23	5.357	1263	1265	1270	rBB	298	202	0.02%	0.003%
24	5.634	1347	1351	1356	rVB	332	241	0.02%	0.003%
25	5.717	1356	1377	1412	rBV2	383986	1058945	100.00%	13.419%
26	5.907	1435	1436	1439	rVB2	548	243	0.02%	0.003%
27	5.975	1451	1457	1461	rVB4	422	510	0.05%	0.006%
28	6.110	1496	1499	1502	rBV3	353	272	0.03%	0.003%
29	6.242	1522	1540	1563	rBV	345586	670156	63.29%	8.492%
30	6.531	1620	1630	1634	rBV6	1481	2393	0.23%	0.030%
31	6.682	1664	1677	1714	rBV	240014	474032	44.76%	6.007%
32	6.856	1727	1731	1733	rBV3	227	167	0.02%	0.002%
33	6.930	1750	1754	1757	rBV2	337	291	0.03%	0.004%
34	7.193	1829	1836	1838	rBV3	718	721	0.07%	0.009%
35	7.280	1855	1863	1869	rBV	194	247	0.02%	0.003%
36	7.319	1869	1875	1879	rBV2	220	225	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022724\
 Data File : VU057951.D
 Acq On : 27 Feb 2024 13:04
 Operator : MD/SY
 Sample : VU0227WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK046

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

37	7.505	1924	1933	1938	rBV	105	171	0.02%	0.002%
38	7.560	1938	1950	1974	rBV	128810	239479	22.61%	3.035%
39	7.695	1990	1992	1995	rBV3	418	319	0.03%	0.004%
40	7.804	2019	2026	2028	rBV3	344	360	0.03%	0.005%
41	7.891	2040	2053	2083	rBV	472901	835971	78.94%	10.593%
42	8.174	2130	2141	2169	rBV	85651	155789	14.71%	1.974%
43	8.354	2193	2197	2200	rVB2	286	219	0.02%	0.003%
44	8.386	2205	2207	2211	rBV3	203	174	0.02%	0.002%
45	8.422	2215	2218	2223	rBV2	190	157	0.01%	0.002%
46	8.467	2229	2232	2235	rBV	336	227	0.02%	0.003%
47	8.627	2272	2282	2331	rBV3	184953	425739	40.20%	5.395%
48	8.888	2360	2363	2368	rVB2	284	212	0.02%	0.003%
49	8.981	2389	2392	2395	rVB2	246	157	0.01%	0.002%
50	9.000	2395	2398	2403	rBV2	377	319	0.03%	0.004%
51	9.065	2417	2418	2423	rBV2	212	180	0.02%	0.002%
52	9.135	2436	2440	2445	rVV2	236	251	0.02%	0.003%
53	9.286	2484	2487	2492	rVB2	202	181	0.02%	0.002%
54	9.319	2492	2497	2499	rBV	248	225	0.02%	0.003%
55	9.412	2512	2526	2559	rBV	474486	827207	78.12%	10.482%
56	9.704	2608	2617	2621	rBV3	399	479	0.05%	0.006%
57	9.746	2626	2630	2635	rVB2	192	167	0.02%	0.002%
58	10.020	2711	2715	2718	rBV2	157	164	0.02%	0.002%
59	10.110	2738	2743	2746	rVV2	204	233	0.02%	0.003%
60	10.180	2761	2765	2769	rBV2	198	184	0.02%	0.002%
61	10.286	2795	2798	2803	rVB	229	186	0.02%	0.002%
62	10.357	2816	2820	2825	rBV2	201	185	0.02%	0.002%
63	10.444	2842	2847	2849	rBV	303	281	0.03%	0.004%
64	10.486	2857	2860	2862	rBV	266	184	0.02%	0.002%
65	10.582	2884	2890	2894	rBV2	287	340	0.03%	0.004%
66	10.749	2930	2942	2964	rBV	268774	445286	42.05%	5.643%
67	10.878	2978	2982	2985	rVB2	265	175	0.02%	0.002%
68	10.904	2986	2990	2992	rBV	181	157	0.01%	0.002%
69	11.068	3038	3041	3045	rBV2	226	162	0.02%	0.002%
70	11.093	3045	3049	3054	rVB2	600	471	0.04%	0.006%
71	11.142	3054	3064	3067	rBV2	262	358	0.03%	0.005%
72	11.183	3072	3077	3081	rBV2	173	196	0.02%	0.002%
73	11.476	3162	3168	3174	rBV3	387	521	0.05%	0.007%
74	11.692	3227	3235	3238	rBV2	238	307	0.03%	0.004%
75	11.746	3248	3252	3258	rVB4	751	872	0.08%	0.011%
76	11.807	3258	3271	3290	rBV	482265	780344	73.69%	9.888%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022724\
 Data File : VU057951.D
 Acq On : 27 Feb 2024 13:04
 Operator : MD/SY
 Sample : VU0227WBL01
 Misc : 5.0mL/MSVOA_U/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK046

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
 Title : VOC Analysis

77	12.029	3337	3340	3344	rVB2	287	231	0.02%	0.003%
78	12.190	3376	3390	3418	rBV	411470	689544	65.12%	8.738%
79	12.441	3463	3468	3471	rBV2	168	168	0.02%	0.002%
80	12.618	3519	3523	3525	rBV	183	172	0.02%	0.002%
81	12.634	3525	3528	3533	rVB2	392	299	0.03%	0.004%
82	12.659	3533	3536	3540	rBV2	227	194	0.02%	0.002%
83	12.733	3553	3559	3561	rBV	312	335	0.03%	0.004%
84	12.823	3582	3587	3590	rBV2	233	200	0.02%	0.003%
85	12.859	3595	3598	3600	rBV	257	171	0.02%	0.002%
86	13.235	3711	3715	3719	rVB2	435	359	0.03%	0.005%
87	13.261	3719	3723	3724	rBV	269	186	0.02%	0.002%
88	13.482	3787	3792	3795	rBV2	249	243	0.02%	0.003%
89	13.643	3838	3842	3845	rBV2	255	198	0.02%	0.003%
90	13.855	3905	3908	3914	rBV2	511	458	0.04%	0.006%
91	14.109	3984	3987	3989	rBV2	434	337	0.03%	0.004%
92	14.174	4003	4007	4011	rVV3	345	315	0.03%	0.004%
93	14.193	4011	4013	4015	rVB2	293	156	0.01%	0.002%
94	14.267	4033	4036	4039	rBV	234	182	0.02%	0.002%
95	14.315	4048	4051	4054	rBV2	328	267	0.03%	0.003%
96	14.373	4066	4069	4072	rVB	347	230	0.02%	0.003%
97	14.566	4127	4129	4132	rVB2	295	166	0.02%	0.002%
98	14.913	4234	4237	4244	rBV3	414	525	0.05%	0.007%
99	15.386	4380	4384	4388	rBV3	389	403	0.04%	0.005%
100	16.360	4684	4687	4690	rBV2	857	693	0.07%	0.009%




Sum of corrected areas: 7891437

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022724\
Data File : VU057951.D
Acq On : 27 Feb 2024 13:04
Operator : MD/SY
Sample : VU0227WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK046

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

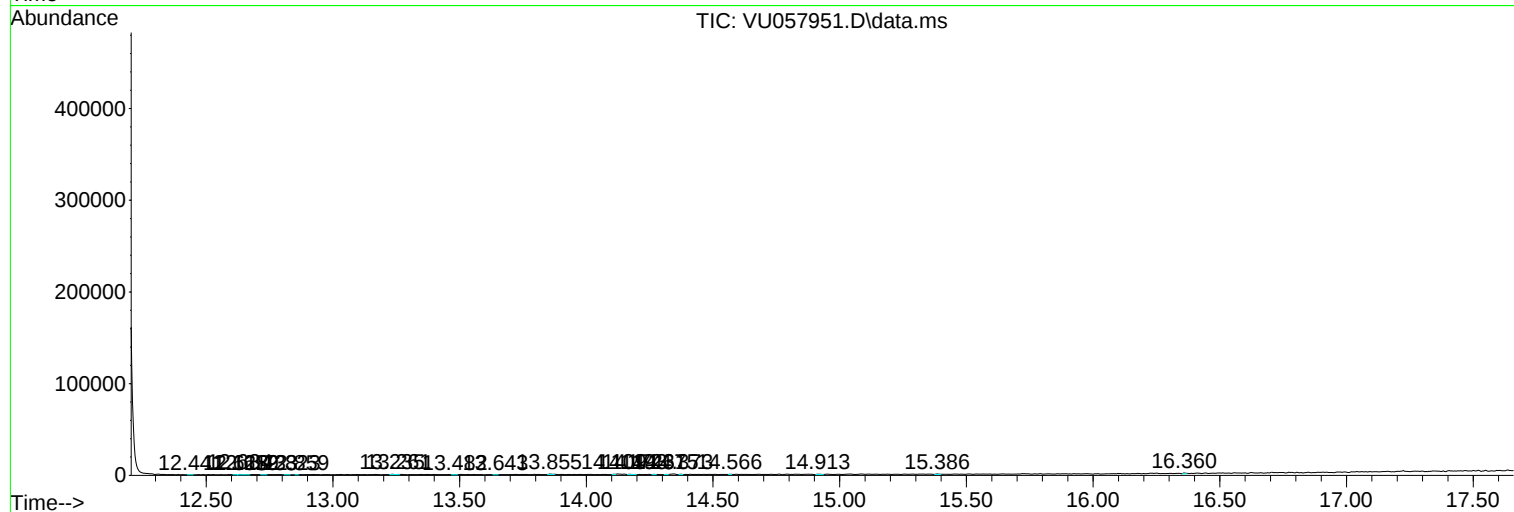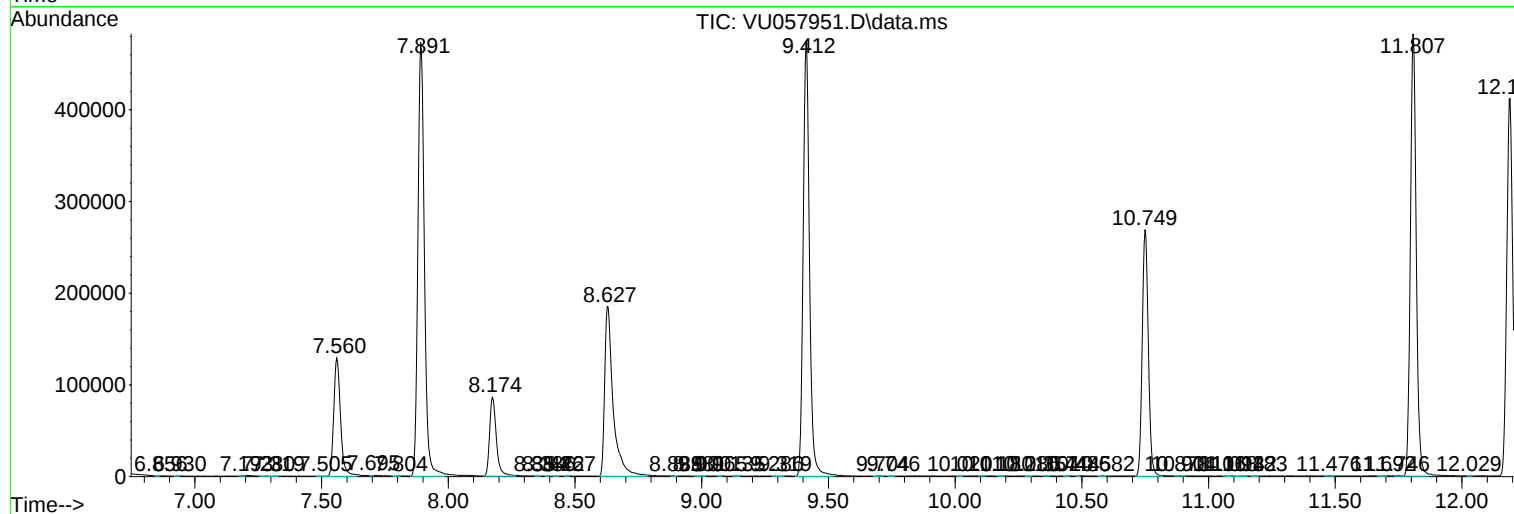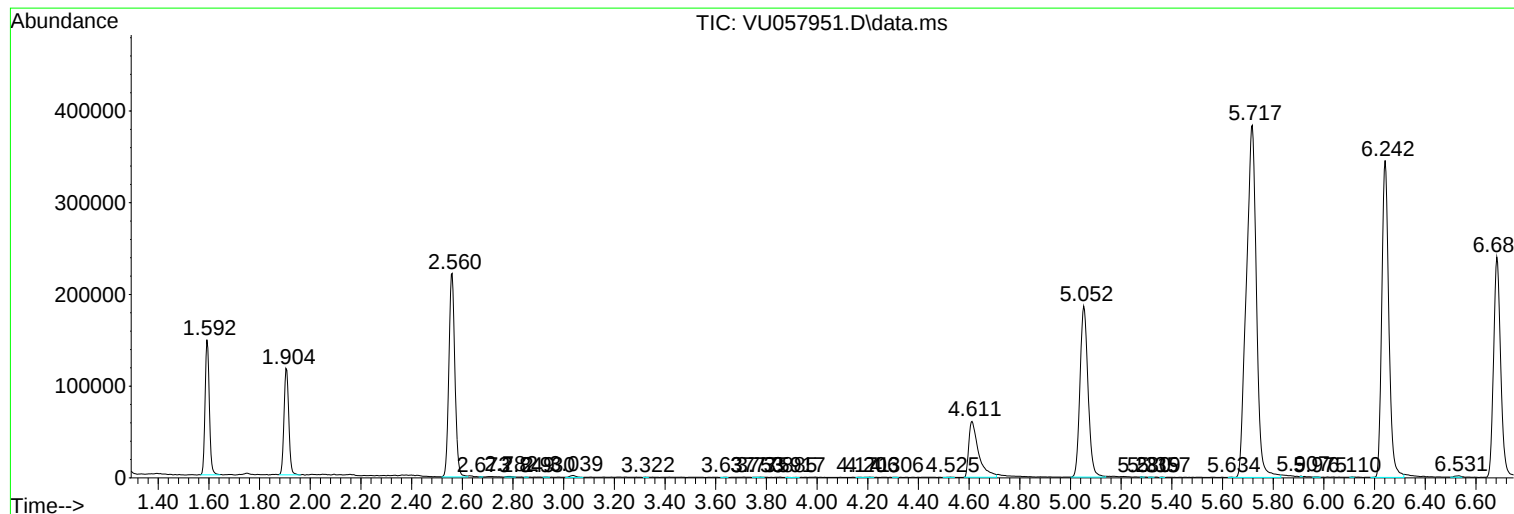

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022724\
Data File : VU057951.D
Acq On : 27 Feb 2024 13:04
Operator : MD/SY
Sample : VU0227WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK046

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022724\
Data File : VU057951.D
Acq On : 27 Feb 2024 13:04
Operator : MD/SY
Sample : VU0227WBL01
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK046

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc