
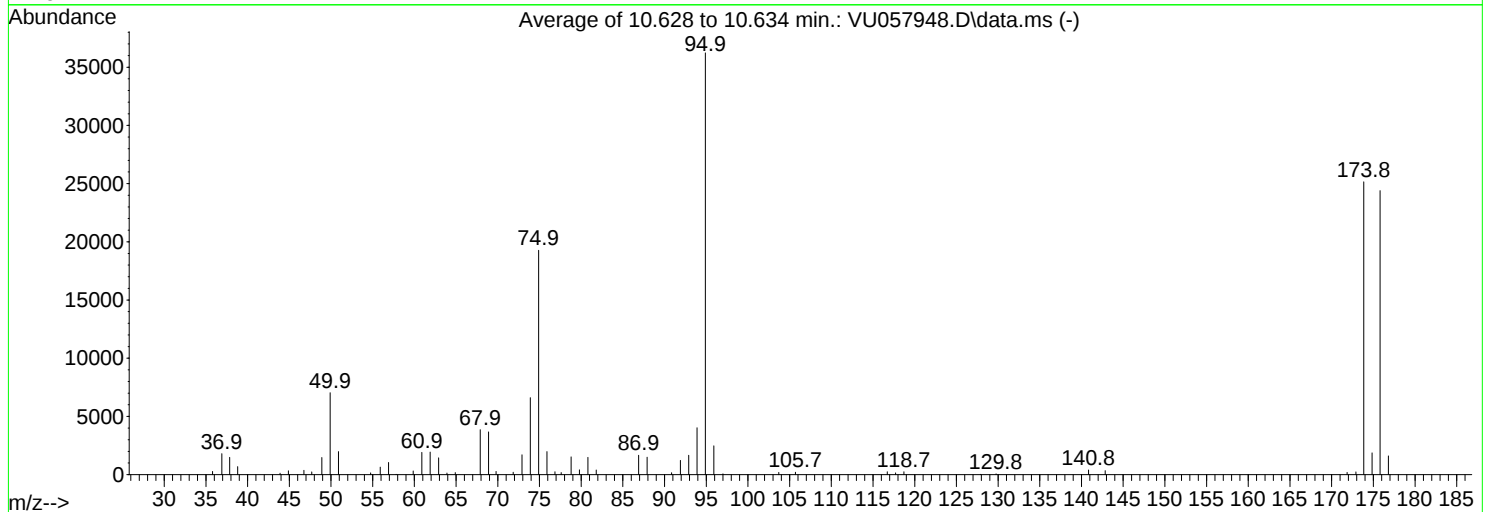


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU022724\
Data File : VU057948.D
Acq On : 27 Feb 2024 08:56
Operator : MD/SY
Sample : BFB044
Misc : 5.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB044

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMULM021924WMA.M
Title : VOC Analysis
Last Update : Wed Feb 28 00:40:01 2024

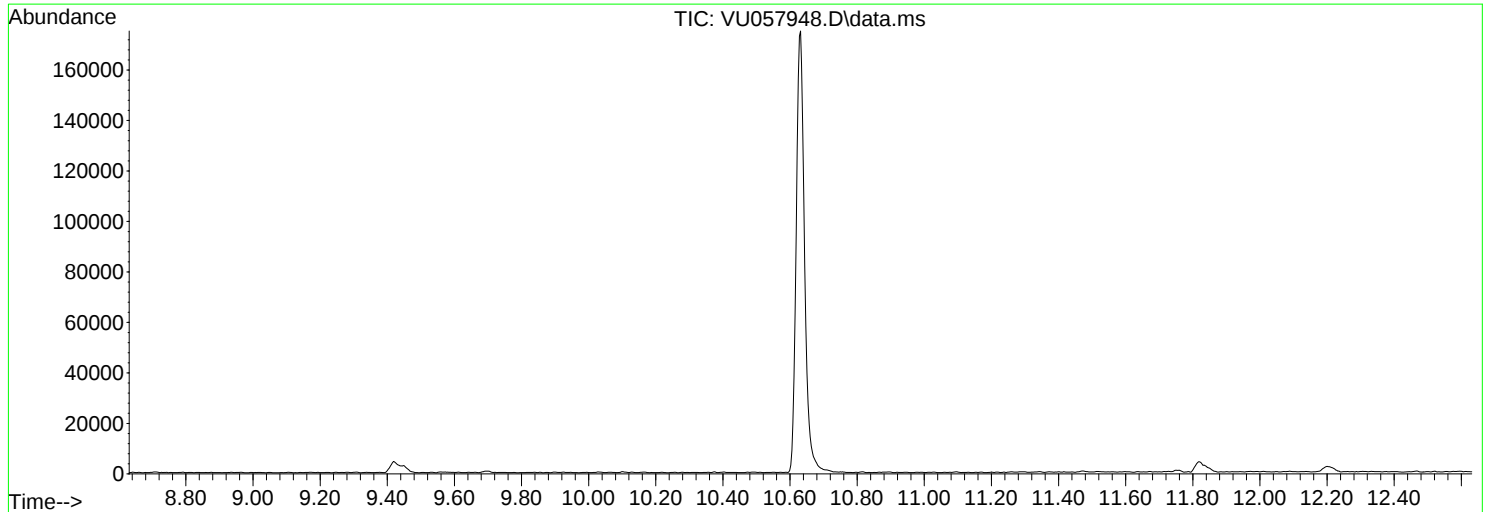

AutoFind: Scans 2904, 2905, 2906; Background Corrected with Scan 2892

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	7037	PASS
75	95	30	80	53.2	19275	PASS
95	95	100	100	100.0	36232	PASS
96	95	5	9	6.8	2474	PASS
173	174	0.00	2	0.9	235	PASS
174	95	50	120	69.4	25155	PASS
175	174	5	9	7.4	1870	PASS
176	174	95	101	97.0	24395	PASS
177	176	5	9	6.6	1602	PASS

m/z	Abundance
39.90	263.0
43.90	379.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044

m/z	Abundance
35.90	261.0
36.90	1808.0
37.90	1590.0
38.80	728.0
39.90	238.0
43.90	487.0
44.90	357.0
46.80	420.0
47.70	213.0
48.90	1488.0
49.90	7292.0
50.90	1999.0
54.70	154.0
55.90	609.0
56.90	1043.0
57.80	101.0
59.90	306.0
60.90	1956.0
61.90	1976.0
62.90	1510.0
63.90	150.0
64.90	167.0
67.90	4087.0
68.90	3706.0
69.80	286.0
71.80	212.0
72.90	1768.0
73.90	7007.0
74.90	19816.0
75.90	1930.0
76.90	255.0
77.60	204.0
78.80	1514.0
79.80	413.0
80.80	1573.0
81.80	361.0
86.90	1629.0
87.90	1468.0
90.90	164.0
91.90	1205.0
92.90	1658.0
93.90	4023.0
94.90	36904.0
95.90	2568.0
97.00	107.0
103.70	176.0
105.70	218.0
116.70	292.0
117.70	196.0
118.70	287.0
127.90	104.0
129.80	116.0
140.90	399.0
142.90	328.0
171.90	181.0
172.80	219.0
173.90	25072.0
174.80	1979.0
175.80	24456.0
176.80	1660.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044

m/z	Abundance
35.80	275.0
36.90	1879.0
37.80	1519.0
38.80	737.0
39.90	227.0
43.90	512.0
44.90	328.0
46.80	390.0
47.70	250.0
48.90	1516.0
49.90	7237.0
50.90	1991.0
54.80	164.0
55.90	691.0
56.90	1069.0
59.80	319.0
60.90	1970.0
61.90	2015.0
62.90	1478.0
63.90	141.0
64.90	193.0
67.90	3996.0
68.90	3790.0
69.80	286.0
71.90	210.0
72.90	1726.0
73.90	6796.0
74.90	19816.0
75.90	2087.0
76.80	241.0
77.60	194.0
78.80	1558.0
79.80	421.0
80.80	1516.0
81.80	412.0
86.90	1682.0
87.90	1551.0
90.80	174.0
91.90	1281.0
92.90	1744.0
93.90	4095.0
94.90	37360.0
95.90	2536.0
97.00	116.0
103.70	190.0
105.70	201.0
116.70	261.0
117.70	165.0
118.70	262.0
129.70	103.0
140.80	404.0
142.80	344.0
171.80	206.0
172.90	224.0
173.80	25808.0
174.90	1899.0
175.80	25192.0
176.80	1656.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044

m/z	Abundance
35.80	280.0
36.90	1717.0
37.80	1331.0
38.80	606.0
39.80	264.0
43.90	495.0
44.90	316.0
46.70	304.0
47.70	252.0
48.90	1397.0
49.90	6581.0
50.90	1955.0
54.80	155.0
55.90	646.0
56.90	1031.0
59.80	309.0
60.90	1799.0
61.90	1819.0
62.90	1355.0
63.90	118.0
64.90	176.0
67.90	3518.0
68.90	3534.0
69.80	243.0
71.90	208.0
72.90	1599.0
73.90	6023.0
74.90	18192.0
75.90	1920.0
76.80	241.0
77.60	152.0
78.80	1505.0
79.80	400.0
80.80	1372.0
81.80	408.0
86.90	1680.0
87.90	1480.0
90.80	164.0
91.90	1182.0
92.90	1579.0
93.90	3965.0
94.90	34432.0
95.90	2319.0
103.70	193.0
105.70	182.0
116.70	191.0
117.70	117.0
118.70	209.0
140.80	389.0
142.80	363.0
171.80	202.0
173.00	262.0
173.80	24584.0
174.90	1731.0
175.80	23536.0
176.80	1491.0

Instrument :
MSVOA_U
ClientSampleId :
BFB044