

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
 Data File : VU047292.D
 Acq On : 02 Mar 2022 15:39
 Operator : SY/MD
 Sample : N1736-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU047292.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	99	rVB	68722	78307	12.65%	1.690%
2	1.919	171	180	199	rBV	53963	74932	12.10%	1.617%
3	2.572	371	383	396	rBV	113355	183286	29.61%	3.956%
4	4.652	1013	1030	1065	rBV	55811	233383	37.70%	5.037%
5	5.067	1144	1159	1179	rBV	94794	209664	33.87%	4.525%
6	5.729	1343	1365	1388	rBV2	192370	497049	80.29%	10.728%
7	6.250	1513	1527	1560	rVB	166522	313772	50.69%	6.772%
8	6.694	1650	1665	1685	rBV	118876	230161	37.18%	4.968%
9	7.568	1924	1937	1952	rBV	68454	120508	19.47%	2.601%
10	7.899	2026	2040	2059	rBV	252239	427002	68.98%	9.216%
11	8.182	2117	2128	2151	rBV	43551	78751	12.72%	1.700%
12	8.475	2208	2219	2230	rBV	8963	15657	2.53%	0.338%
13	8.636	2255	2269	2297	rBV	335140	619039	100.00%	13.361%
14	9.417	2499	2512	2533	rBV	253290	417368	67.42%	9.009%
15	10.758	2917	2929	2948	rVB	110638	176134	28.45%	3.802%
16	10.893	2961	2971	2984	rBV	10222	16515	2.67%	0.356%
17	11.812	3244	3257	3274	rBV	324538	507801	82.03%	10.960%
18	12.192	3362	3375	3391	rVB	263139	425565	68.75%	9.185%
19	12.774	3545	3556	3565	rBV	5176	8143	1.32%	0.176%




Sum of corrected areas: 4633037

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
Data File : VU047292.D
Acq On : 02 Mar 2022 15:39
Operator : SY/MD
Sample : N1736-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

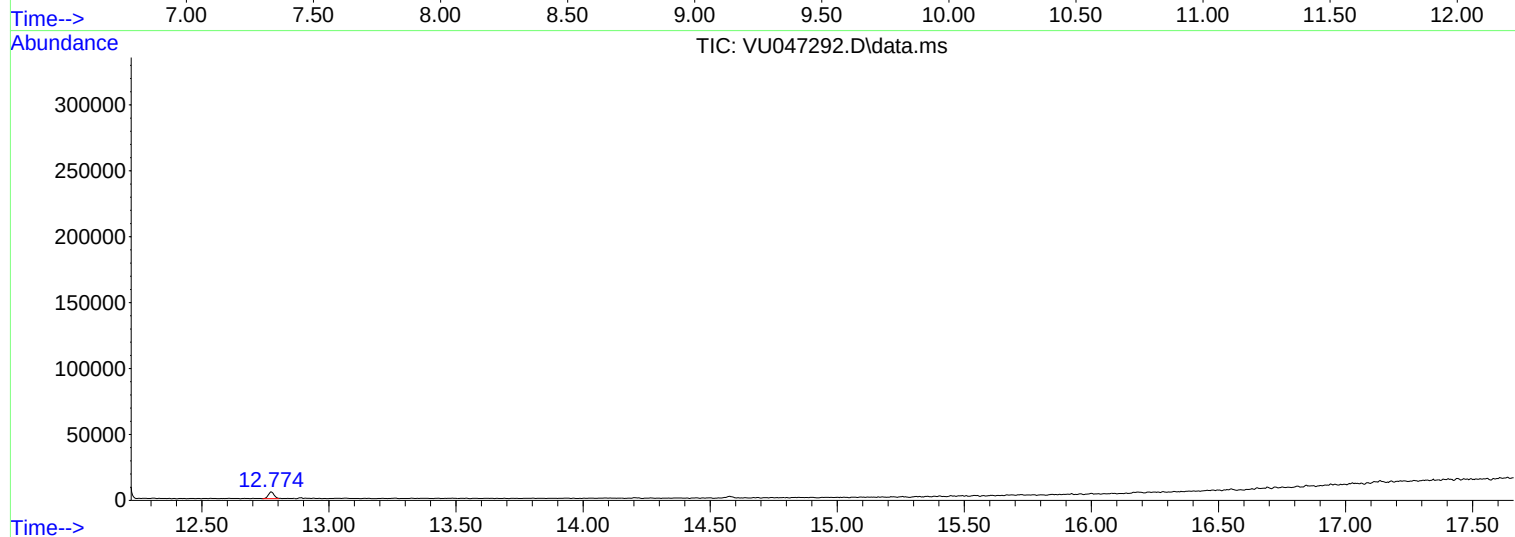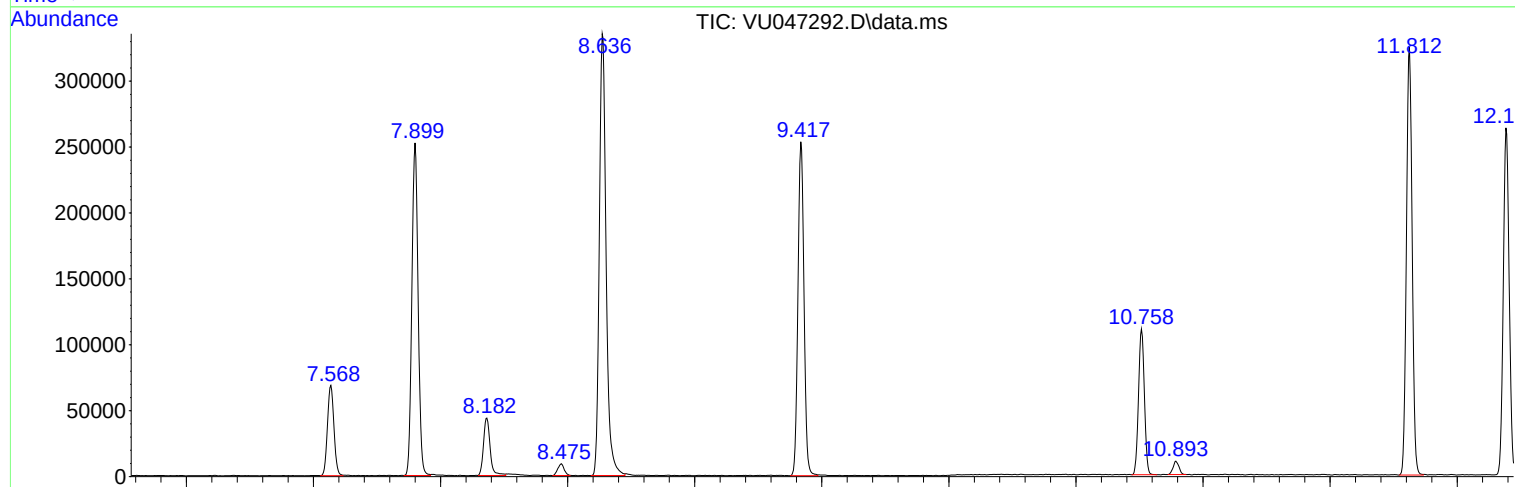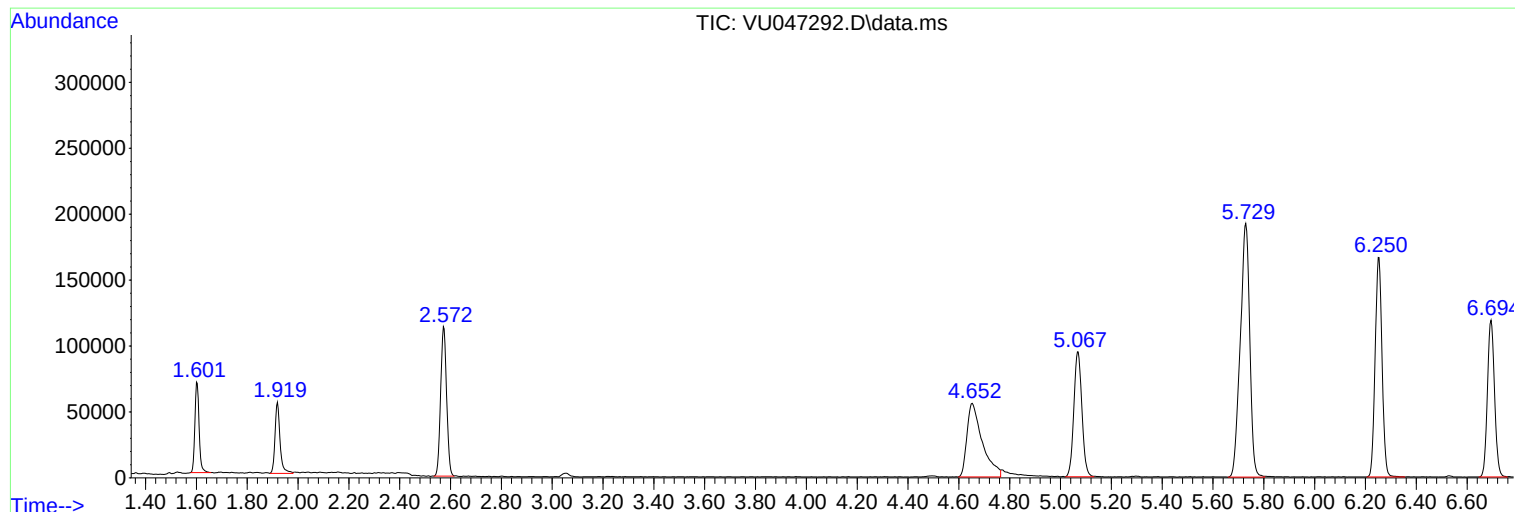

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
Data File : VU047292.D
Acq On : 02 Mar 2022 15:39
Operator : SY/MD
Sample : N1736-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
Data File : VU047292.D
Acq On : 02 Mar 2022 15:39
Operator : SY/MD
Sample : N1736-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
