

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
 Data File : VU047293.D
 Acq On : 02 Mar 2022 16:02
 Operator : SY/MD
 Sample : N1745-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AA0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU047293.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	35	42	53	rBV2	34691	46939	7.25%	0.957%
2	1.600	74	81	97	rBV	70283	81536	12.59%	1.663%
3	1.919	171	180	199	rBV	55429	74618	11.52%	1.522%
4	2.575	371	384	397	rBV	118247	190006	29.33%	3.876%
5	4.649	1011	1029	1074	rBV	61157	258808	39.95%	5.279%
6	5.067	1143	1159	1188	rVB	98569	215574	33.28%	4.397%
7	5.729	1342	1365	1384	rBV2	198750	511613	78.97%	10.436%
8	6.250	1513	1527	1548	rBV	175515	329180	50.81%	6.715%
9	6.693	1647	1665	1683	rBV	121980	238393	36.80%	4.863%
10	7.169	1802	1813	1824	rVB7	3398	6688	1.03%	0.136%
11	7.568	1919	1937	1951	rBV	71216	123089	19.00%	2.511%
12	7.716	1972	1983	1996	rBV3	15118	27314	4.22%	0.557%
13	7.899	2027	2040	2058	rBV	261348	446089	68.86%	9.099%
14	8.182	2116	2128	2149	rBV	45626	81735	12.62%	1.667%
15	8.475	2209	2219	2229	rBV	4091	7080	1.09%	0.144%
16	8.636	2256	2269	2298	rBV	353539	647824	100.00%	13.215%
17	9.417	2499	2512	2538	rBV	265868	438989	67.76%	8.955%
18	10.758	2917	2929	2942	rBV	115075	182850	28.23%	3.730%
19	10.896	2960	2972	2983	rBV2	7698	13313	2.06%	0.272%
20	11.812	3245	3257	3272	rBV	344586	539335	83.25%	11.002%
21	12.195	3360	3376	3391	rVB	274636	441377	68.13%	9.003%




Sum of corrected areas: 4902350

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
Data File : VU047293.D
Acq On : 02 Mar 2022 16:02
Operator : SY/MD
Sample : N1745-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

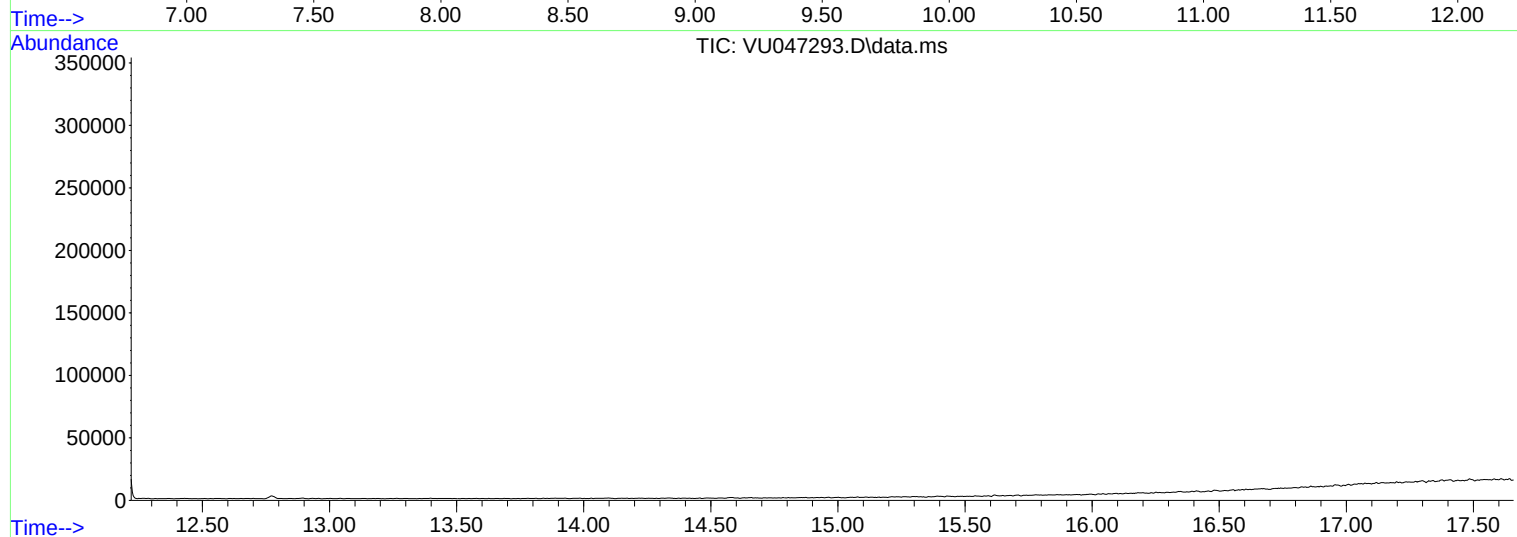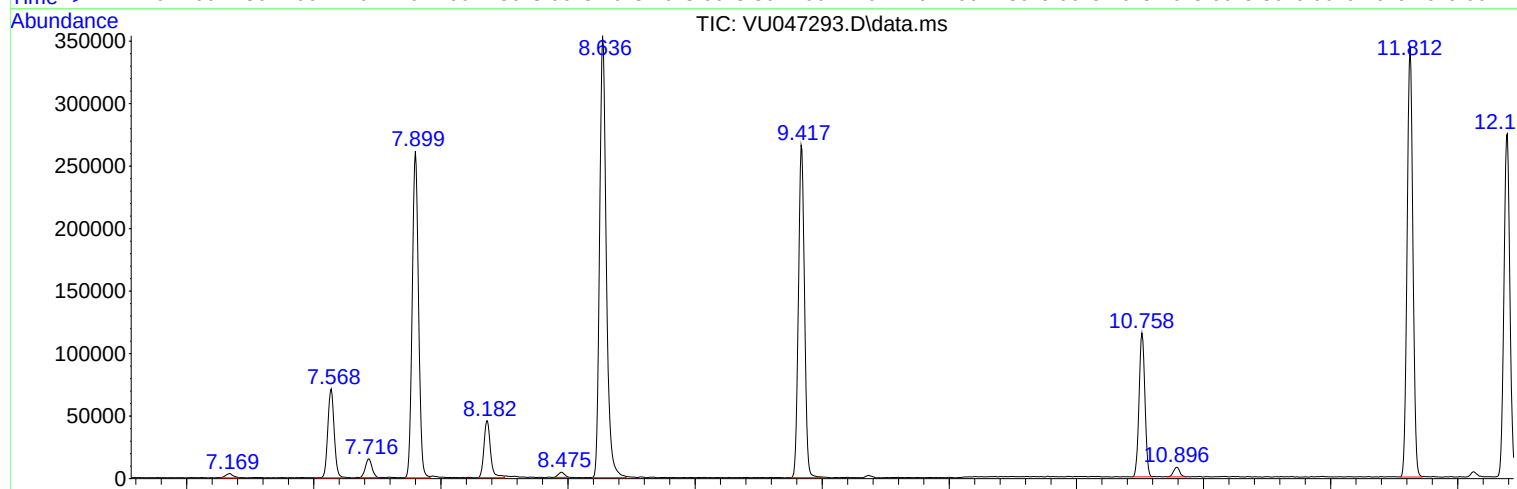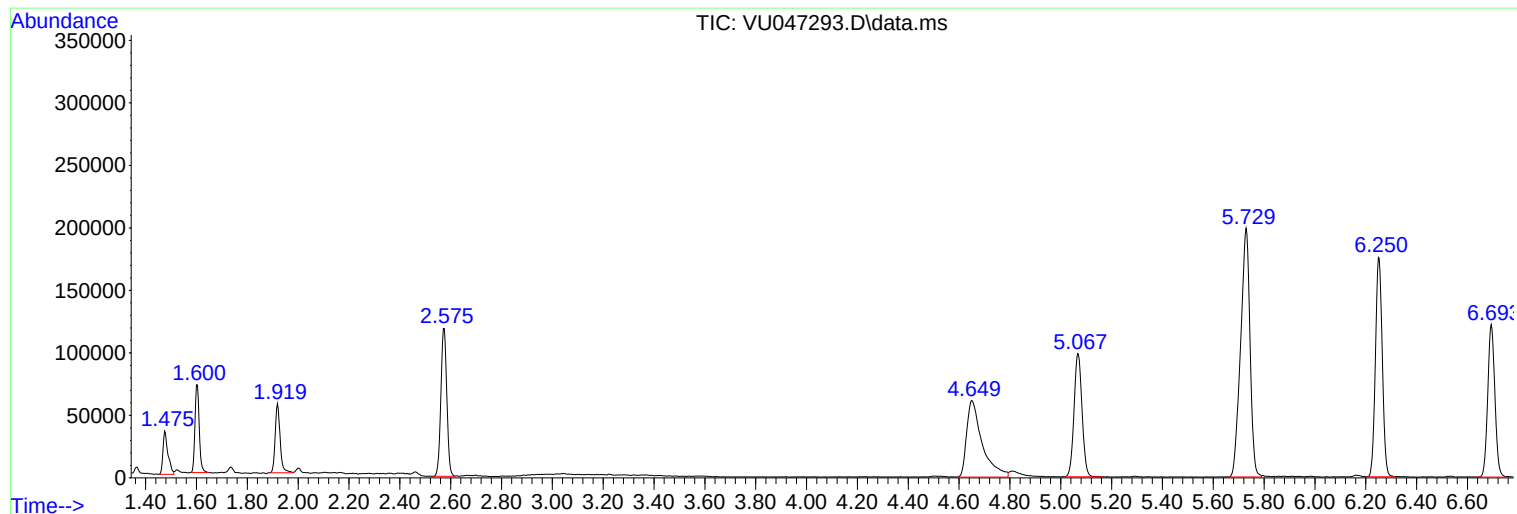

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
Data File : VU047293.D
Acq On : 02 Mar 2022 16:02
Operator : SY/MD
Sample : N1745-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AA0










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Cyclic1.475 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
1.475	0.71 ug/L	46939	1,4-Difluorobenzene	6.253

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Cyclopropane	42	C3H6	000075-19-4	90
2			Cyclopropane	42	C3H6	000075-19-4	90
3			Propene	42	C3H6	000115-07-1	83
4			Cyclopropane	42	C3H6	000075-19-4	53
5			Cyclopropene	40	C3H4	002781-85-3	10

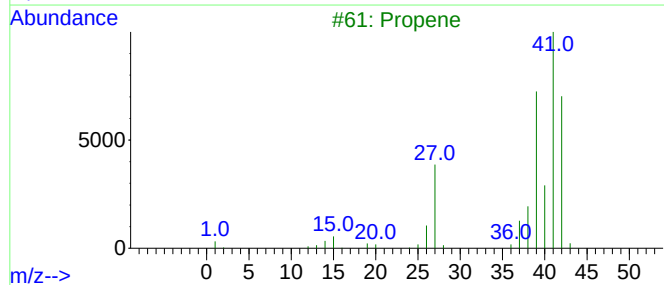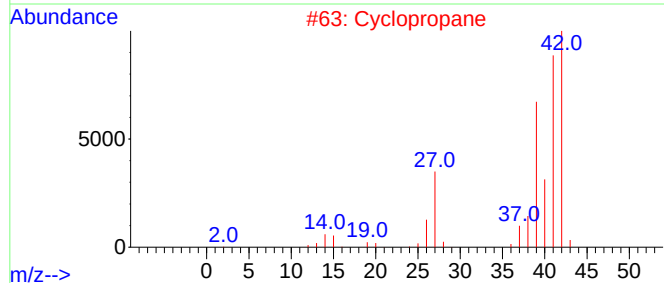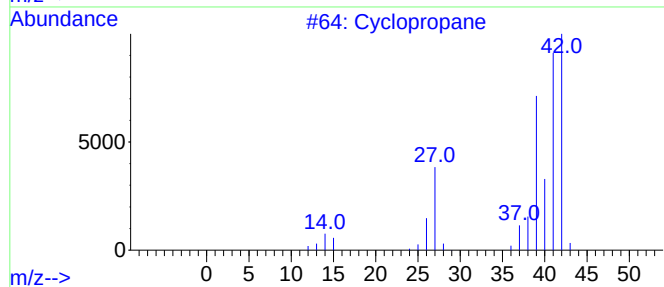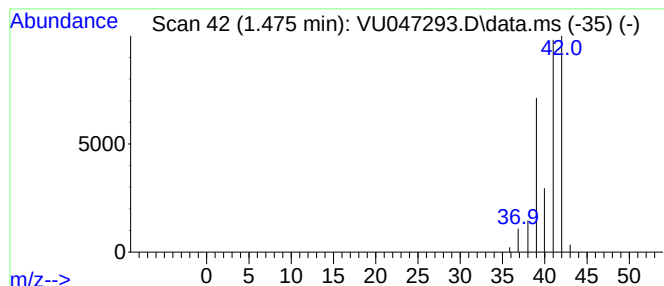

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
Data File : VU047293.D
Acq On : 02 Mar 2022 16:02
Operator : SY/MD
Sample : N1745-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AA0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: C...	1.475	0.7	ug/L	46939	1	6.253	329180	5.0