

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
 Data File : VU047296.D
 Acq On : 02 Mar 2022 17:13
 Operator : SY/MD
 Sample : N1745-04
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AA4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU047296.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	36	42	50	rBV2	6053	7612	1.21%	0.161%
2	1.526	52	58	68	rVB	8233	10527	1.67%	0.222%
3	1.604	74	82	99	rBV	66109	77822	12.33%	1.644%
4	1.919	171	180	196	rBV	52534	70487	11.17%	1.489%
5	2.459	339	348	362	rVB	29877	48943	7.76%	1.034%
6	2.571	371	383	398	rVB	111253	181918	28.83%	3.843%
7	4.652	1012	1030	1071	rBV	58468	253470	40.17%	5.355%
8	5.066	1144	1159	1182	rBV	92417	202737	32.13%	4.283%
9	5.729	1343	1365	1385	rBV2	190881	490666	77.76%	10.366%
10	6.250	1514	1527	1543	rBV	171098	318705	50.50%	6.733%
11	6.693	1651	1665	1685	rBV	116945	228249	36.17%	4.822%
12	7.169	1802	1813	1827	rVB2	6170	12986	2.06%	0.274%
13	7.568	1922	1937	1952	rBV	66591	117001	18.54%	2.472%
14	7.716	1970	1983	1995	rBV2	10892	19695	3.12%	0.416%
15	7.899	2025	2040	2056	rBV	245650	422179	66.90%	8.919%
16	8.182	2117	2128	2150	rBV2	42565	76944	12.19%	1.626%
17	8.635	2253	2269	2296	rBV	346579	631039	100.00%	13.332%
18	9.417	2499	2512	2532	rBV	255652	425039	67.36%	8.980%
19	10.758	2917	2929	2943	rVB	113011	175689	27.84%	3.712%
20	10.896	2959	2972	2982	rBV2	6810	11914	1.89%	0.252%
21	11.812	3245	3257	3278	rBV	332774	520627	82.50%	10.999%
22	12.063	3327	3335	3350	rVB4	4038	7227	1.15%	0.153%
23	12.195	3363	3376	3390	rBV	263049	421882	66.86%	8.913%




Sum of corrected areas: 4733358

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
Data File : VU047296.D
Acq On : 02 Mar 2022 17:13
Operator : SY/MD
Sample : N1745-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

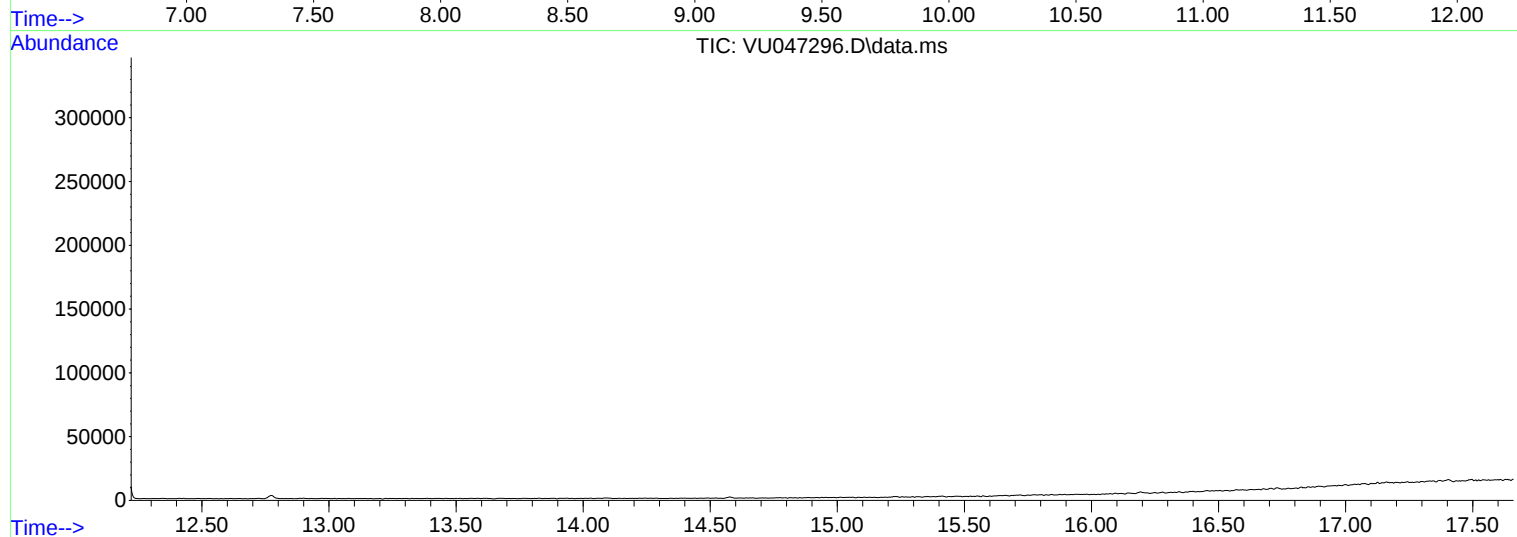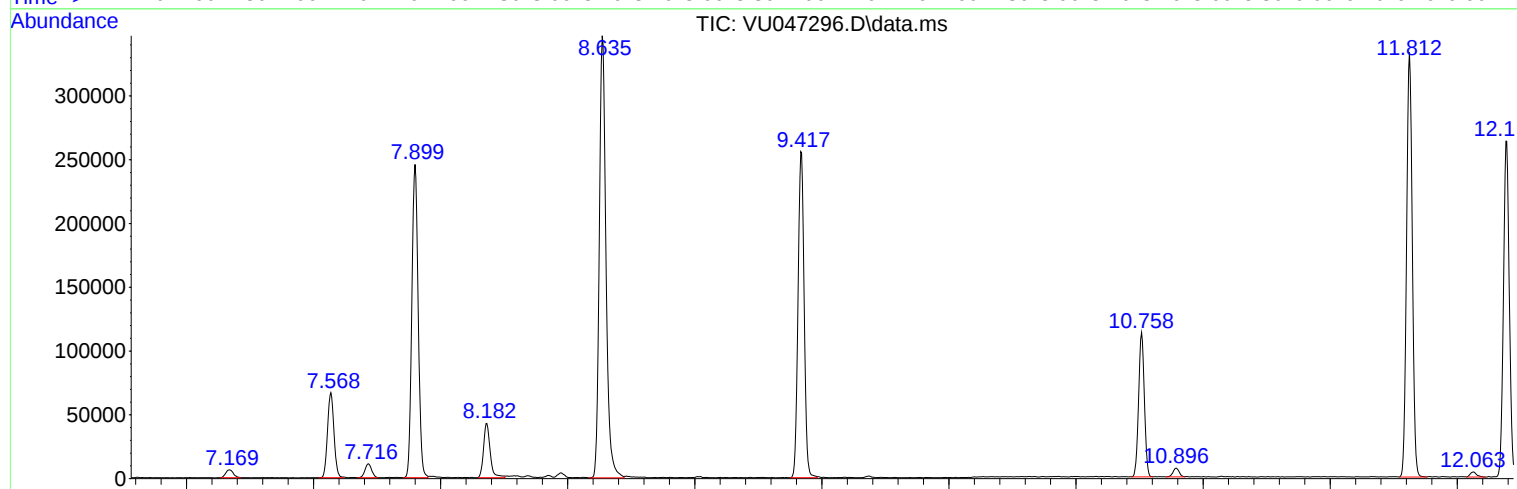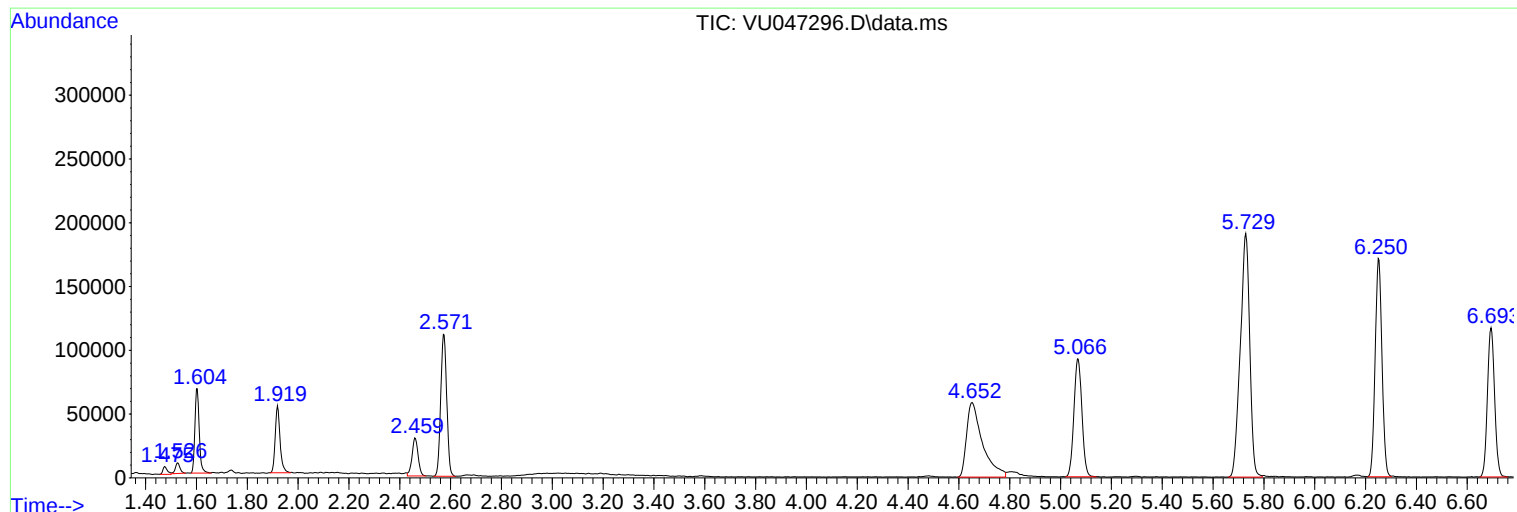

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
Data File : VU047296.D
Acq On : 02 Mar 2022 17:13
Operator : SY/MD
Sample : N1745-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AA4










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.459	0.77 ug/L	48943	1,4-Difluorobenzene	6.250

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	80
2			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	58
3			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	53
4			Bis(2-chloroethyl) sulfone	190	C4H8Cl2O2S	000471-03-4	9
5			Propanoic acid, 2-chloro-	108	C3H5ClO2	000598-78-7	9

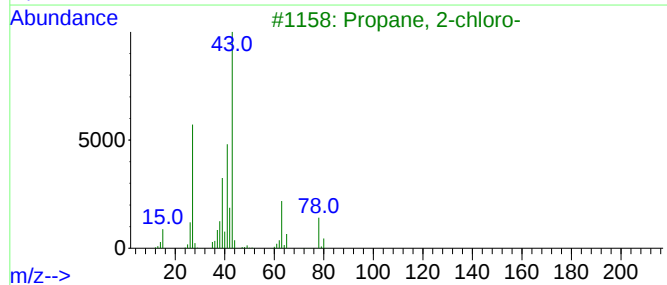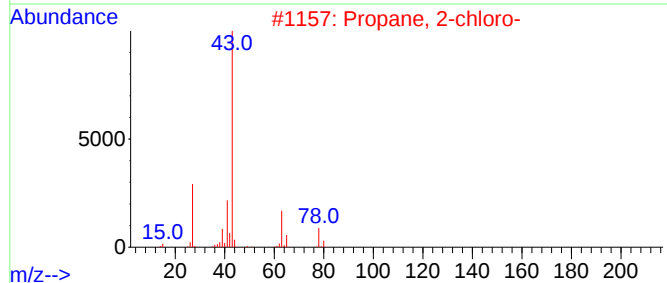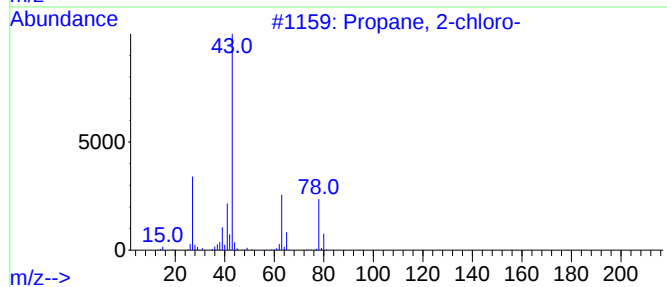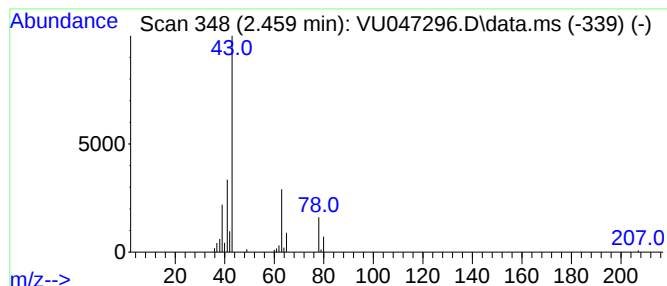

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
Data File : VU047296.D
Acq On : 02 Mar 2022 17:13
Operator : SY/MD
Sample : N1745-04
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.459	0.8	ug/L	48943	1	6.250	318705	5.0