

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
 Data File : VU047297.D
 Acq On : 02 Mar 2022 17:37
 Operator : SY/MD
 Sample : N1745-05
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AA5

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047297.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.363	3	7	17	rVB4	5909	6555	1.03%	0.139%
2	1.475	35	42	53	rBV2	23274	29646	4.67%	0.631%
3	1.600	73	81	94	rBV	69992	81856	12.88%	1.741%
4	1.919	171	180	198	rVB	53015	73092	11.50%	1.555%
5	2.571	372	383	397	rBV	111267	181296	28.53%	3.856%
6	4.649	1013	1029	1072	rBV2	60666	254376	40.04%	5.410%
7	5.070	1139	1160	1186	rBV	95907	215225	33.87%	4.578%
8	5.729	1343	1365	1391	rBV2	191420	494290	77.80%	10.513%
9	6.250	1511	1527	1547	rBV	169591	317974	50.05%	6.763%
10	6.693	1651	1665	1684	rBV	119207	230463	36.27%	4.902%
11	7.568	1924	1937	1953	rBV	62822	109038	17.16%	2.319%
12	7.713	1971	1982	1993	rBV3	8310	15730	2.48%	0.335%
13	7.899	2026	2040	2060	rBV	246665	424230	66.77%	9.023%
14	8.182	2116	2128	2142	rBV	39330	68442	10.77%	1.456%
15	8.636	2254	2269	2300	rBV	351074	635353	100.00%	13.514%
16	9.417	2499	2512	2531	rBV	260049	424069	66.75%	9.020%
17	10.758	2917	2929	2942	rBV	110137	176144	27.72%	3.747%
18	10.893	2961	2971	2984	rBV	7197	12116	1.91%	0.258%
19	11.812	3245	3257	3279	rBV	329359	512332	80.64%	10.897%
20	12.063	3326	3335	3348	rBV2	7902	13046	2.05%	0.277%
21	12.192	3364	3375	3394	rVB	266299	426275	67.09%	9.067%




Sum of corrected areas: 4701548

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
Data File : VU047297.D
Acq On : 02 Mar 2022 17:37
Operator : SY/MD
Sample : N1745-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

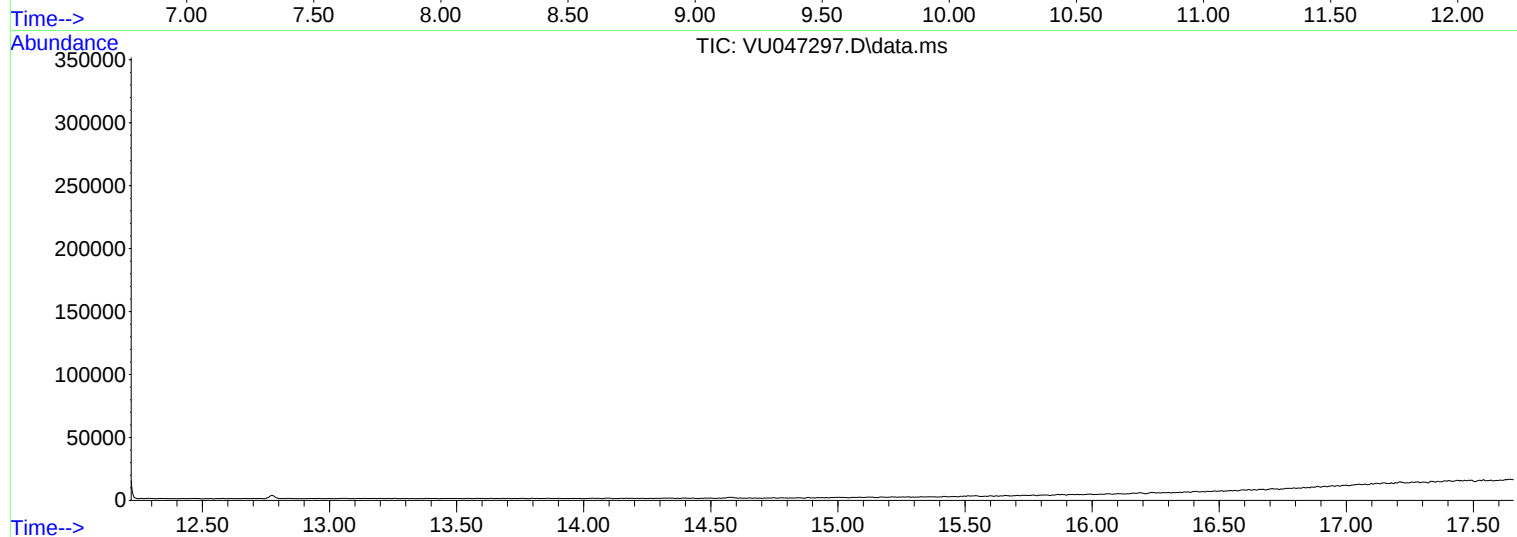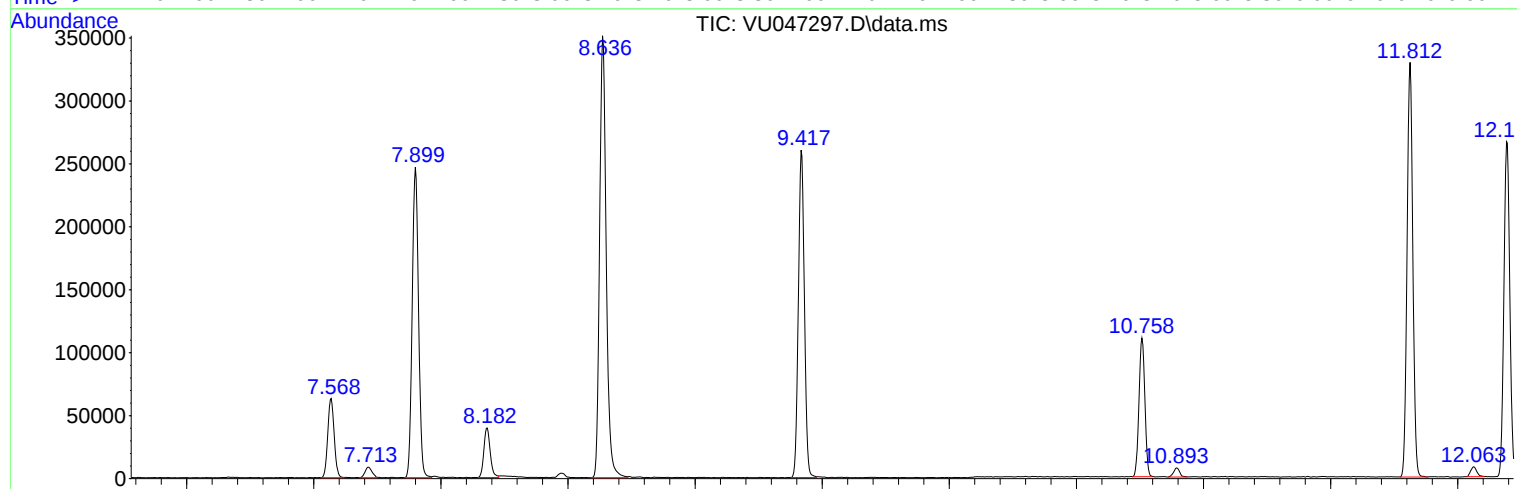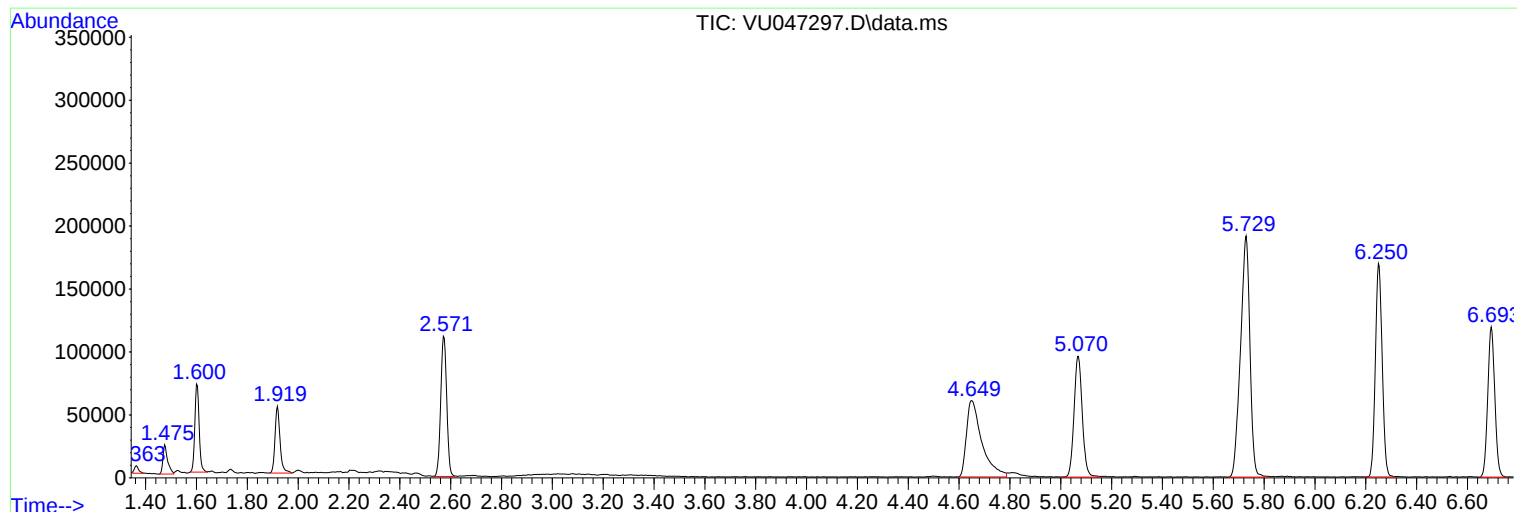

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
Data File : VU047297.D
Acq On : 02 Mar 2022 17:37
Operator : SY/MD
Sample : N1745-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
Data File : VU047297.D
Acq On : 02 Mar 2022 17:37
Operator : SY/MD
Sample : N1745-05
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AA5

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc