

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
 Data File : VU047302.D
 Acq On : 02 Mar 2022 19:34
 Operator : SY/MD
 Sample : N1745-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 H0AB0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047302.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.475	36	42	52	rBV2	6286	9059	1.47%	0.193%
2	1.527	52	58	67	rVV	6639	9242	1.50%	0.197%
3	1.601	74	81	102	rVB	69095	79546	12.88%	1.696%
4	1.736	116	123	132	rVB	11925	15014	2.43%	0.320%
5	1.919	171	180	195	rBV	52806	72301	11.71%	1.541%
6	2.459	339	348	363	rVB	26066	43596	7.06%	0.929%
7	2.572	369	383	398	rBV	112105	182620	29.57%	3.893%
8	4.649	1012	1029	1072	rBV	54424	226088	36.61%	4.820%
9	5.067	1143	1159	1182	rBV	93247	203717	32.99%	4.343%
10	5.729	1343	1365	1388	rBV2	189064	490973	79.50%	10.466%
11	6.250	1513	1527	1552	rBV	166792	316165	51.19%	6.740%
12	6.694	1651	1665	1686	rBV	118396	228709	37.03%	4.876%
13	7.166	1801	1812	1825	rBV3	6006	11900	1.93%	0.254%
14	7.568	1925	1937	1952	rBV	63867	112322	18.19%	2.394%
15	7.716	1970	1983	1995	rBV3	10756	20192	3.27%	0.430%
16	7.899	2026	2040	2061	rBV	245938	420789	68.14%	8.970%
17	8.182	2116	2128	2145	rBV2	40301	71678	11.61%	1.528%
18	8.472	2209	2218	2232	rVB	4591	8285	1.34%	0.177%
19	8.636	2256	2269	2307	rBV	313024	617579	100.00%	13.165%
20	9.417	2500	2512	2541	rBV	253053	420023	68.01%	8.954%
21	10.758	2917	2929	2945	rVB	109813	175912	28.48%	3.750%
22	10.893	2961	2971	2988	rVB	9845	16440	2.66%	0.350%
23	11.812	3244	3257	3273	rBV	325398	508394	82.32%	10.838%
24	12.063	3327	3335	3346	rBV3	4156	6781	1.10%	0.145%
25	12.195	3360	3376	3391	rBV	259859	423645	68.60%	9.031%




Sum of corrected areas: 4690970

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
Data File : VU047302.D
Acq On : 02 Mar 2022 19:34
Operator : SY/MD
Sample : N1745-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

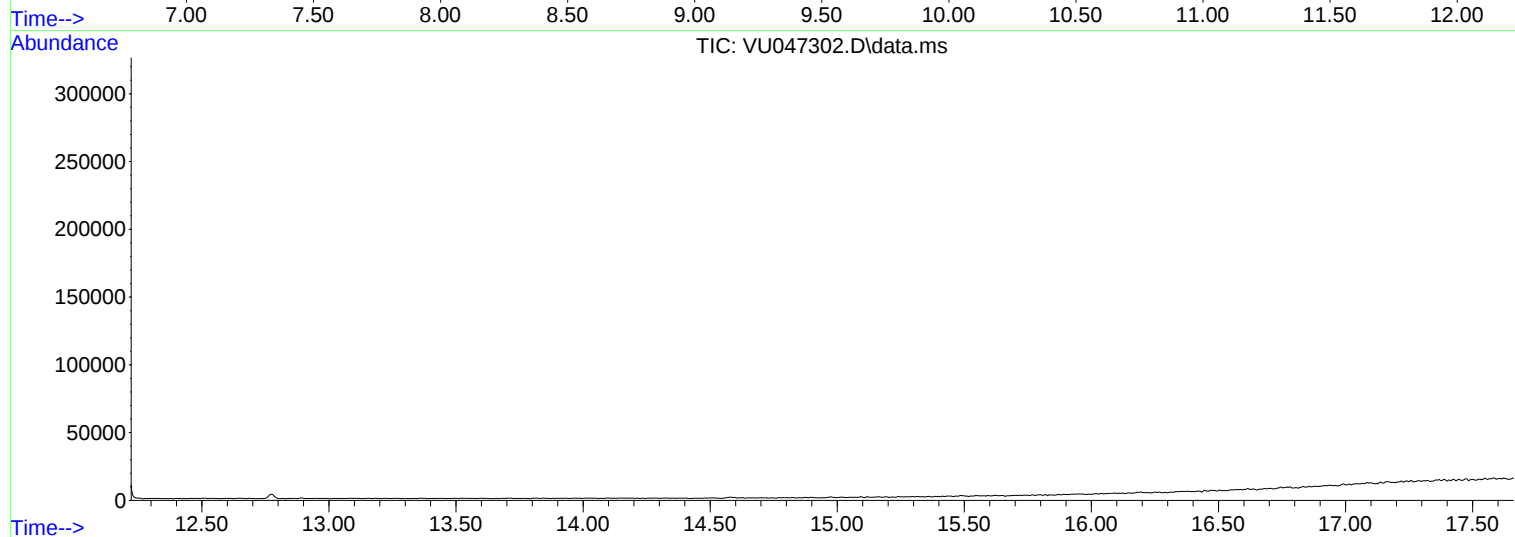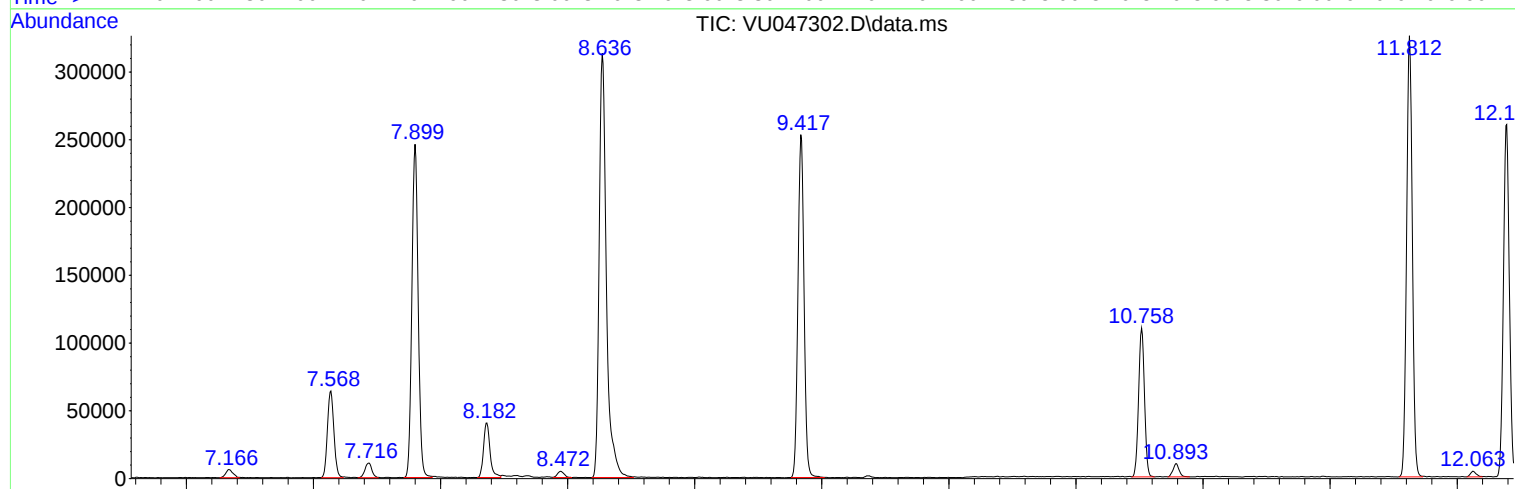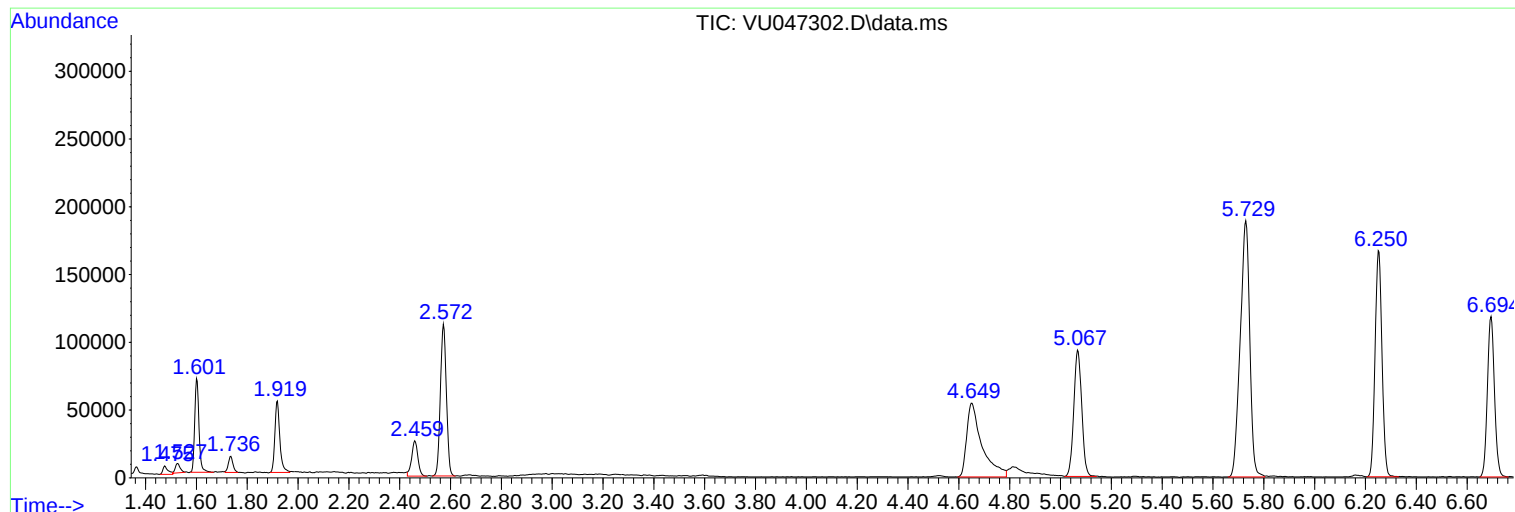

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
Data File : VU047302.D
Acq On : 02 Mar 2022 19:34
Operator : SY/MD
Sample : N1745-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB0










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Propane, 2-chloro- Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.459	0.69 ug/L	43596	1,4-Difluorobenzene	6.253

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	90
2			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	78
3			Propane, 2-chloro-	78	C3H7Cl	000075-29-6	72
4			2-(2'-Chloroethoxy)-propene	120	C5H9ClO	099586-46-6	9
5			Propanoic acid, 2-chloro-	108	C3H5ClO2	000598-78-7	9

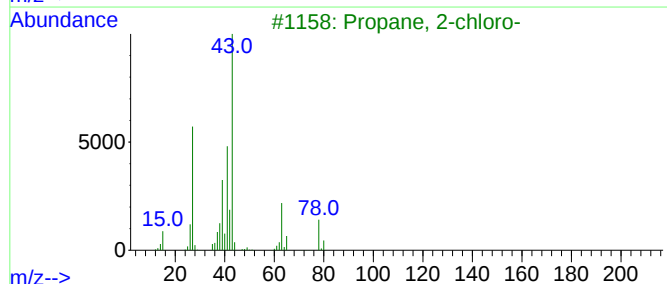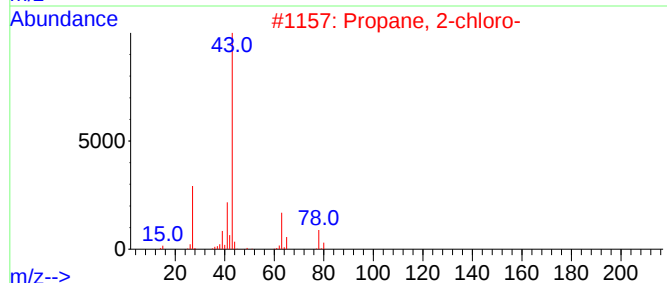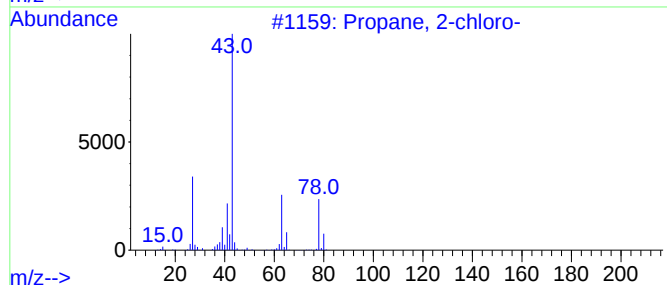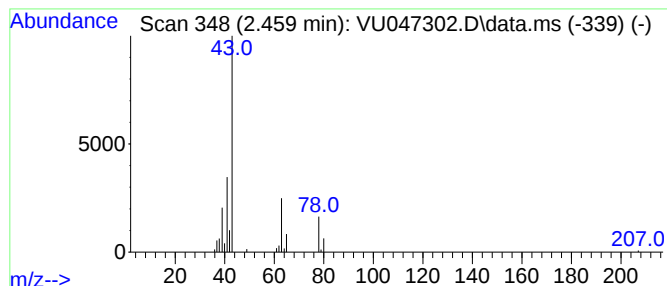

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
Data File : VU047302.D
Acq On : 02 Mar 2022 19:34
Operator : SY/MD
Sample : N1745-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
H0AB0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Propane, 2-chloro-	2.459	0.7	ug/L	43596	1	6.253	316165	5.0