


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030222\
 Data File : VU047284.D
 Acq On : 02 Mar 2022 08:48
 Operator : SY/MD
 Sample : BFB059
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFB059

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Fri Mar 04 01:50:04 2022

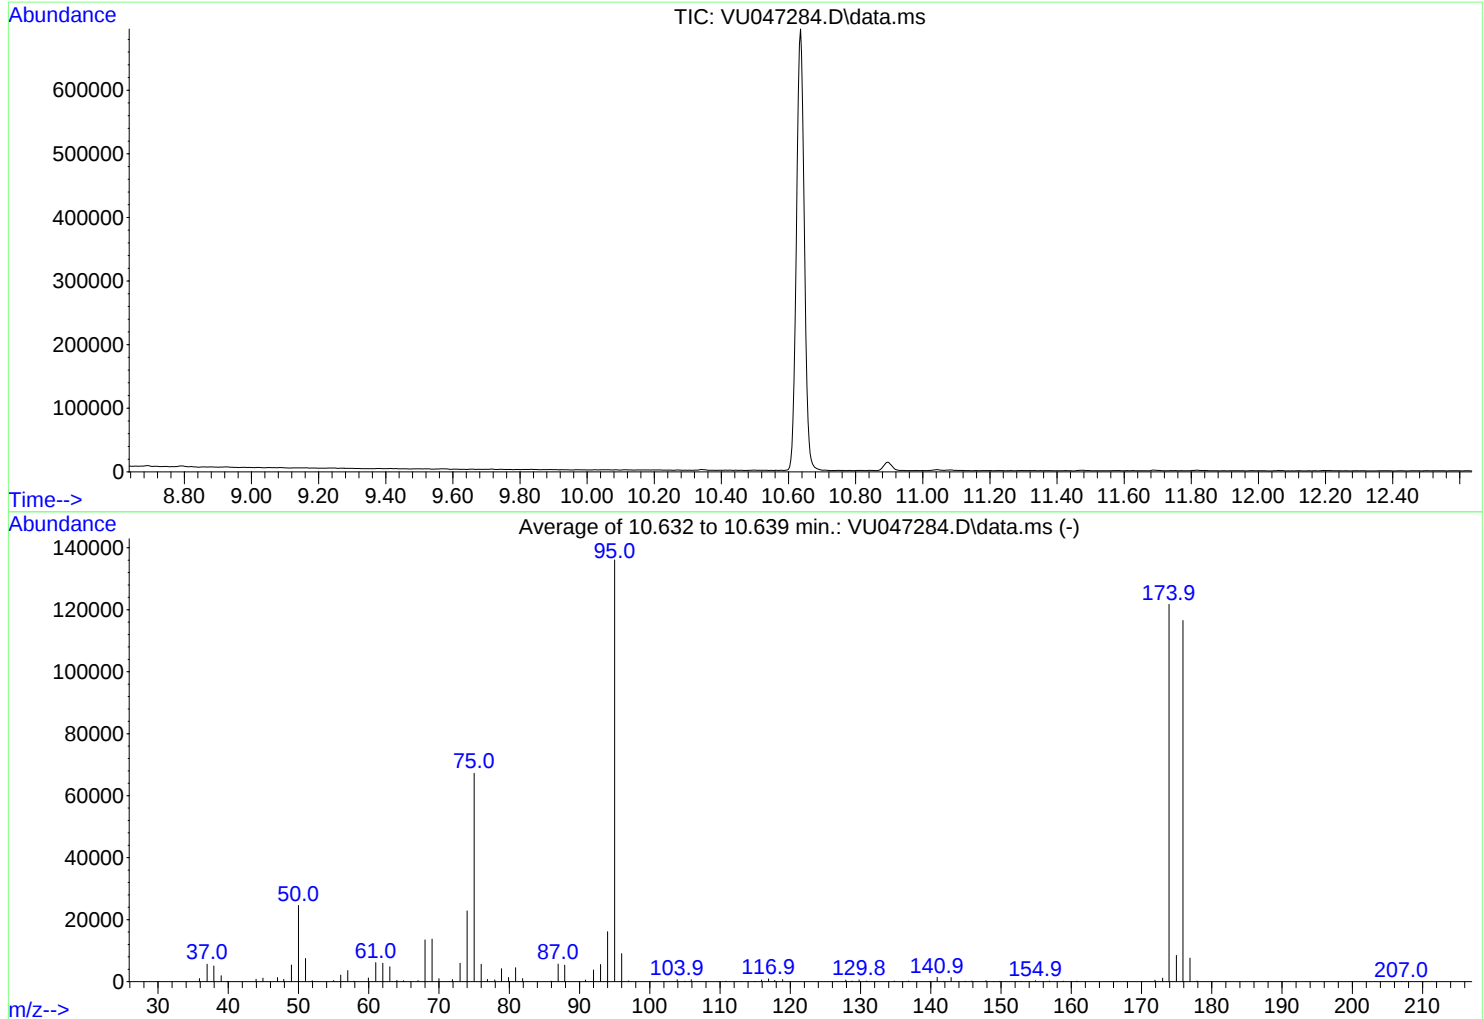

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	24560	PASS
75	95	30	80	49.4	67240	PASS
95	95	100	100	100.0	136107	PASS
96	95	5	9	6.6	9050	PASS
173	174	0.00	2	0.9	1115	PASS
174	95	50	120	89.4	121723	PASS
175	174	5	9	7.0	8495	PASS
176	174	95	101	95.7	116541	PASS
177	176	5	9	6.5	7577	PASS

m/z	Abundance
35.90	1325.0
37.90	479.0
39.90	254.0
43.90	336.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

m/z	Abundance
36.00	2356.0
37.00	5762.0
38.00	5521.0
39.00	1940.0
39.90	328.0
44.00	1115.0
45.00	1189.0
46.00	103.0
47.00	1322.0
47.90	729.0
49.00	5544.0
50.00	25056.0
51.00	7597.0
52.00	329.0
55.00	359.0
56.00	2062.0
57.00	3607.0
57.90	187.0
60.00	1229.0
61.00	6132.0
62.00	5970.0
63.00	4771.0
64.00	421.0
64.90	324.0
67.00	339.0
68.00	13635.0
69.00	13818.0
70.00	1041.0
71.90	690.0
73.00	6010.0
74.00	23080.0
75.00	67648.0
76.00	5844.0
76.90	741.0
78.00	559.0
78.90	4298.0
79.90	1396.0
80.90	4553.0
81.90	906.0
86.00	153.0
86.90	5531.0
87.90	5483.0
90.80	523.0
92.00	3737.0
93.00	5563.0
94.00	16108.0
95.00	135744.0
96.00	9284.0
97.00	296.0
103.90	618.0
105.00	157.0
105.90	583.0
110.80	155.0
115.00	139.0
115.90	515.0
116.90	920.0
117.80	416.0
118.90	690.0
127.90	501.0
128.80	212.0
129.80	581.0
130.90	197.0
134.80	206.0
136.80	194.0
139.80	116.0
140.90	1262.0
141.80	113.0
142.90	1338.0
144.90	125.0
145.90	201.0
147.90	287.0
149.80	126.0
152.90	121.0
154.90	279.0
156.90	214.0
158.90	195.0
160.80	171.0
171.90	516.0
173.00	1150.0
173.90	119056.0
174.90	8473.0
175.90	113864.0
176.90	7359.0
177.90	210.0
207.00	118.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

m/z	Abundance
35.00	2321.0
37.00	5755.0
38.00	5693.0
39.00	1982.0
39.00	349.0
44.00	1138.0
45.00	1180.0
47.00	1357.0
47.00	758.0
49.00	5561.0
50.00	25256.0
51.00	7729.0
51.00	318.0
55.00	361.0
56.00	2195.0
57.00	3637.0
57.00	186.0
60.00	1279.0
61.00	6339.0
62.00	6107.0
63.00	4995.0
64.00	413.0
64.00	317.0
67.00	395.0
68.00	13949.0
69.00	14155.0
70.00	988.0
71.00	659.0
73.00	6090.0
74.00	23464.0
75.00	69312.0
76.00	5763.0
76.00	738.0
77.00	580.0
78.00	4326.0
79.00	1421.0
80.00	4629.0
81.00	1004.0
85.00	145.0
87.00	5826.0
87.00	5487.0
90.00	507.0
92.00	3916.0
93.00	5691.0
94.00	16552.0
95.00	140160.0
96.00	9328.0
97.00	287.0
103.00	640.0
105.00	149.0
105.00	616.0
109.00	100.0
110.00	150.0
113.00	111.0
114.00	122.0
115.00	533.0
116.00	946.0
117.00	426.0
118.00	705.0
127.00	540.0
128.00	241.0
129.00	604.0
130.00	224.0
134.00	240.0
136.00	197.0
139.00	120.0
140.00	1440.0
141.00	112.0
142.00	1400.0
144.00	139.0
145.00	215.0
147.00	305.0
149.00	134.0
152.00	129.0
154.00	361.0
156.00	191.0
158.00	173.0
160.00	162.0
171.00	498.0
173.00	1127.0
173.00	125552.0
175.00	8763.0
175.00	120112.0
176.00	7802.0
177.00	213.0
207.00	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059

m/z	Abundance
35.90	2216.0
37.00	5323.0
38.00	5397.0
39.00	1899.0
39.90	368.0
44.00	1057.0
44.90	1066.0
47.00	1165.0
47.90	724.0
49.00	5085.0
50.00	23368.0
51.00	7189.0
51.90	294.0
55.00	321.0
56.00	2112.0
57.00	3420.0
57.90	172.0
59.90	1123.0
61.00	5898.0
62.00	5694.0
63.00	4703.0
64.00	386.0
65.00	275.0
67.00	392.0
68.00	12901.0
69.00	13230.0
70.00	930.0
71.90	616.0
73.00	5712.0
74.00	21888.0
75.00	64760.0
76.00	5269.0
76.90	717.0
77.90	516.0
78.90	3923.0
79.90	1303.0
80.90	4310.0
81.90	973.0
85.90	123.0
87.00	5614.0
87.90	5007.0
90.90	462.0
92.00	3651.0
93.00	5341.0
94.00	15644.0
95.00	132416.0
96.00	8538.0
97.00	232.0
103.90	604.0
105.00	135.0
105.90	601.0
109.80	105.0
110.90	123.0
114.90	115.0
115.90	507.0
116.90	867.0
117.80	408.0
118.90	646.0
127.90	479.0
128.80	249.0
129.80	521.0
130.90	245.0
134.80	235.0
136.90	177.0
140.90	1437.0
141.90	135.0
142.90	1329.0
144.90	147.0
145.80	208.0
147.90	289.0
148.90	109.0
149.70	110.0
152.80	120.0
154.90	386.0
156.90	197.0
158.80	139.0
160.80	148.0
171.90	462.0
173.00	1068.0
173.90	120560.0
175.00	8248.0
175.90	115648.0
176.90	7571.0
177.90	219.0

Instrument :
MSVOA_U
ClientSampleId :
BFB059