




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
 Data File : VU047313.D
 Acq On : 03 Mar 2022 14:24
 Operator : SY/MD
 Sample : N1773-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFY11

Manual IntegrationsAPPROVED

Quant Time: Mar 04 01:55:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 04 01:50:04 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/04/2022
 Supervised By :Mahesh Dadoda 03/04/2022

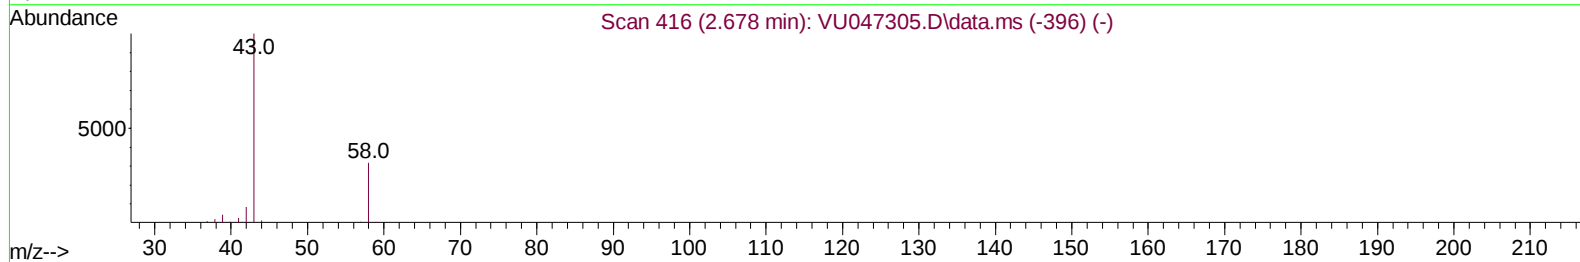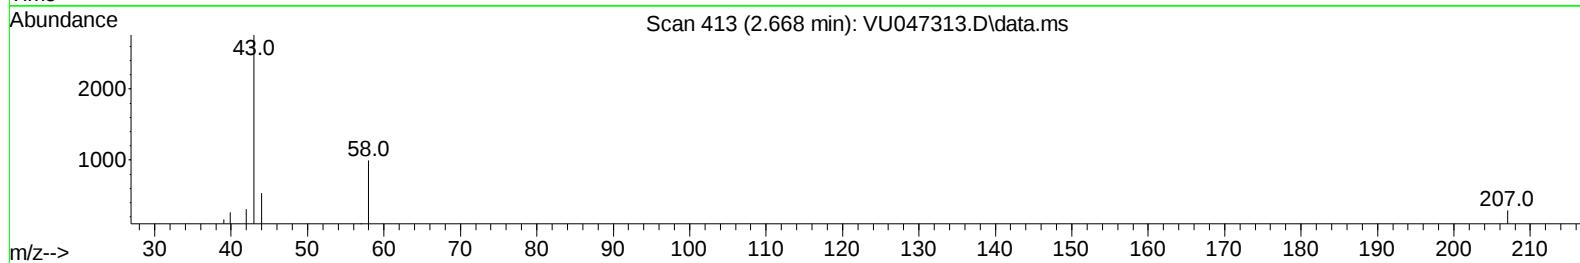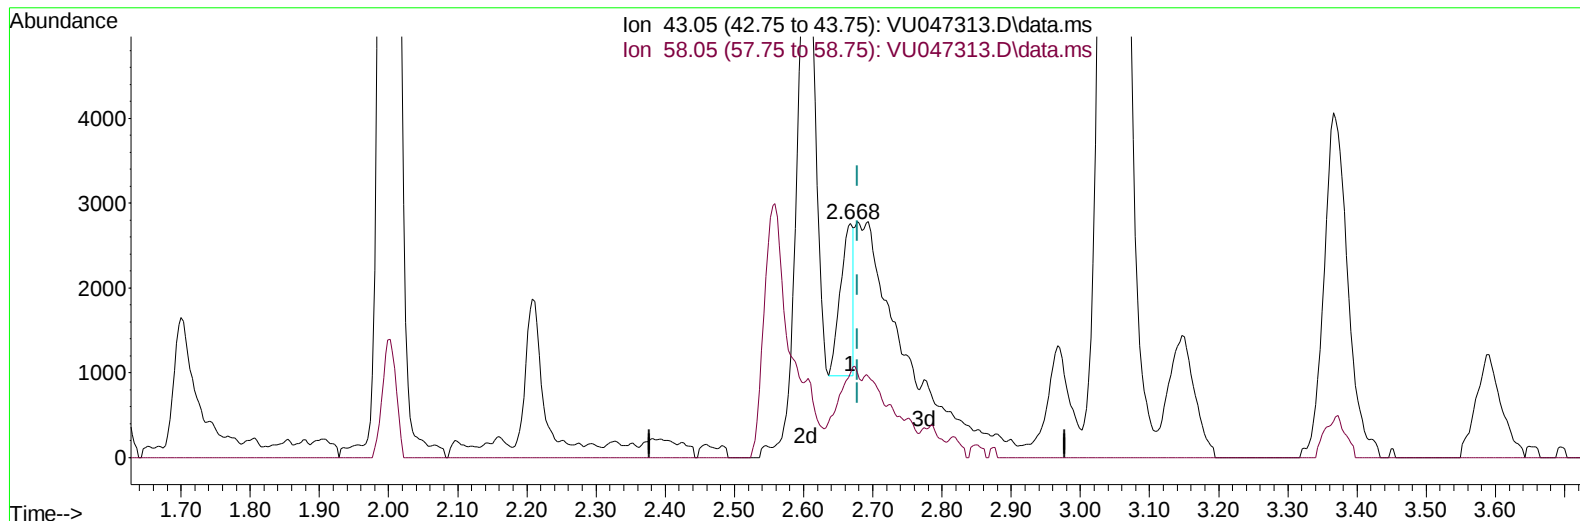

TIC: VU047313.D\data.ms

(13) Acetone (T)

2.668min (-0.010) 1.59 ug/L

response 2312

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	61.68
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
 Data File : VU047313.D
 Acq On : 03 Mar 2022 14:24
 Operator : SY/MD
 Sample : N1773-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFY11

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/04/2022
 Supervised By :Mahesh Dadoda 03/04/2022

Quant Time: Mar 04 01:55:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 04 01:50:04 2022
 Response via : Initial Calibration

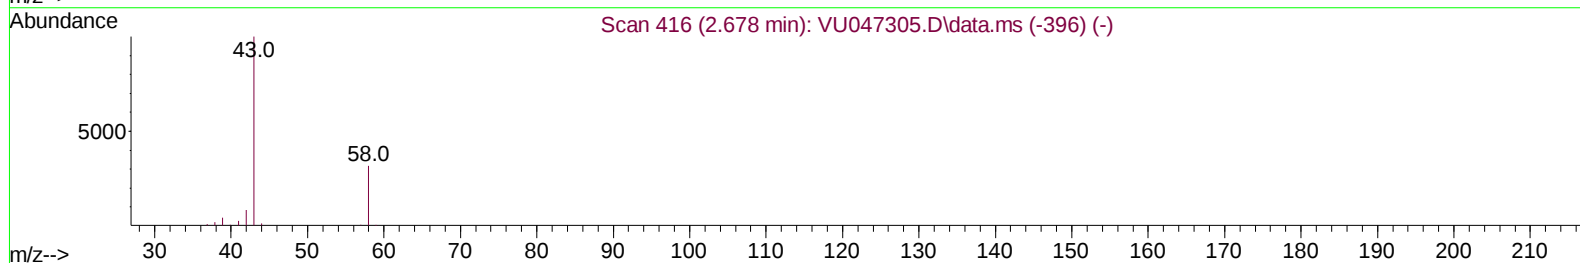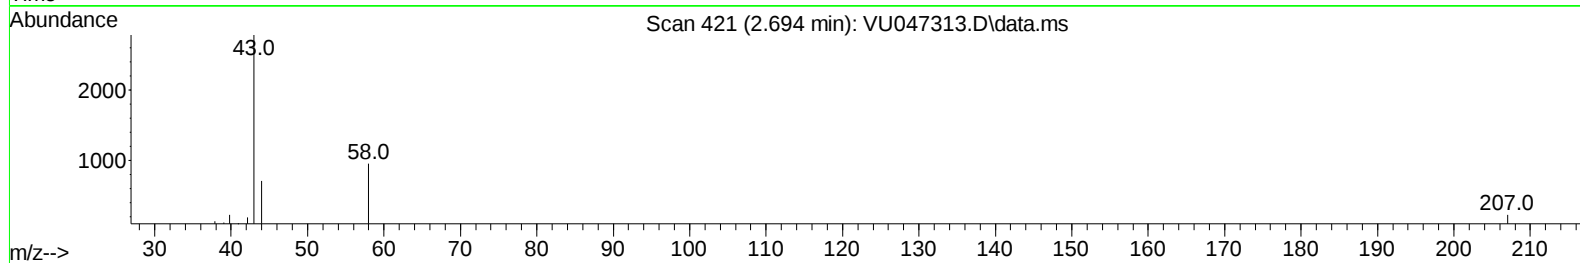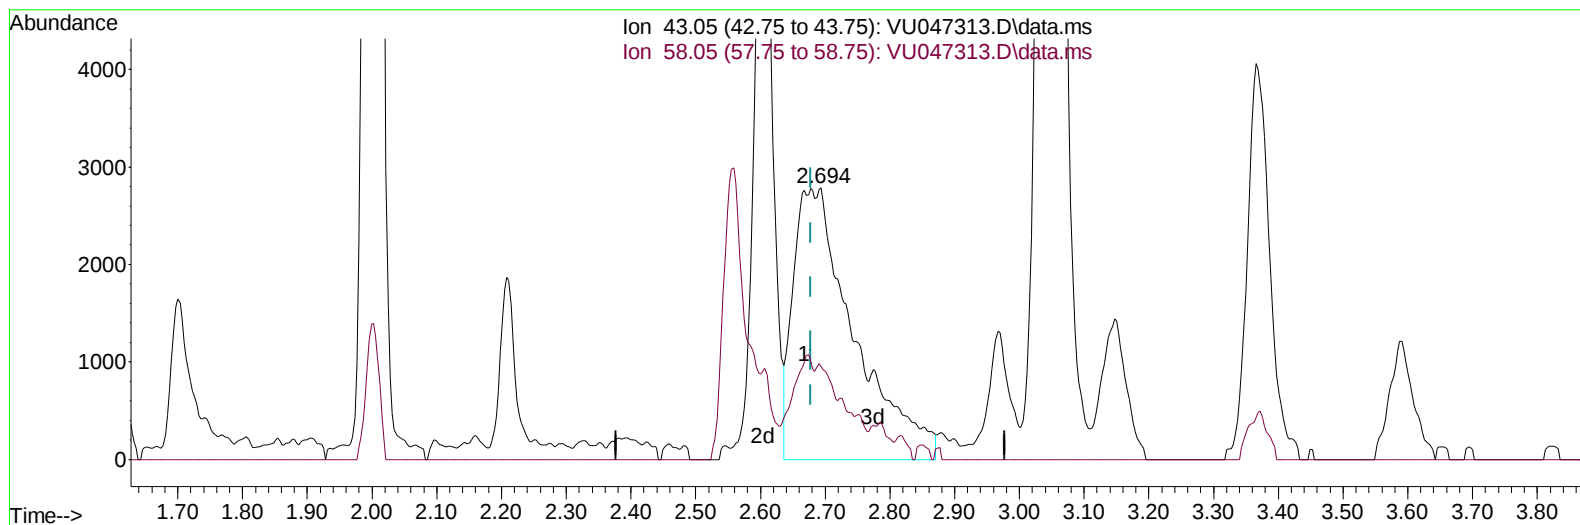

TIC: VU047313.D\data.ms

(13) Acetone (T)

2.694min (+ 0.016) 12.52 ug/L m

response 18144

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	7.86
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
 Data File : VU047313.D
 Acq On : 03 Mar 2022 14:24
 Operator : SY/MD
 Sample : N1773-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFY11

Manual IntegrationsAPPROVED

Quant Time: Mar 04 01:55:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 04 01:50:04 2022
 Response via : Initial Calibration

Reviewed By : John Carlone 03/04/2022
 Supervised By : Mahesh Dadoda 03/04/2022

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	6.253	114		143455	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.417	117		147836	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152		91848	5.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	1.600	65		45000	3.714	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130		Recovery	=	74.200%	
7) Chloroethane-d5	1.919	69		37749	3.931	ug/L	0.00
Spiked Amount 5.000	Range 65	- 130		Recovery	=	78.600%	
11) 1,1-Dichloroethene-d2	2.571	65		19534	3.898	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125		Recovery	=	78.000%	
20) 2-Butanone-d5	4.649	46		152150	52.540	ug/L	0.00
Spiked Amount 50.000	Range 40	- 130		Recovery	=	105.080%	
24) Chloroform-d	5.070	84		86331	4.290	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	85.800%	
26) 1,2-Dichloroethane-d4	5.706	65		47267	4.224	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	84.400%	
32) Benzene-d6	5.732	84		174199	4.217	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125		Recovery	=	84.400%	
36) 1,2-Dichloropropane-d6	6.693	67		56143	4.271	ug/L	0.00
Spiked Amount 5.000	Range 60	- 140		Recovery	=	85.400%	
41) Toluene-d8	7.899	98		163643	4.050	ug/L	0.00
Spiked Amount 5.000	Range 70	- 130		Recovery	=	81.000%	
43) trans-1,3-Dichloroprop...	8.182	79		24284	4.076	ug/L	0.00
Spiked Amount 5.000	Range 55	- 130		Recovery	=	81.600%	
46) 2-Hexanone-d5	8.636	63		131257	41.839	ug/L	0.00
Spiked Amount 50.000	Range 45	- 130		Recovery	=	83.680%	
56) 1,1,2,2-Tetrachloroeth...	10.758	84		52662	4.408	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120		Recovery	=	88.200%	
66) 1,2-Dichlorobenzene-d4	12.195	152		72651	4.409	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120		Recovery	=	88.200%	
Target Compounds							
						Qvalue	
13) Acetone	2.694	43		18144m	12.515	ug/L	
17) Methyl tert-butyl Ether	3.369	73		36808	1.427	ug/L #	57
19) 1,1-Dichloroethane	3.874	63		2477	0.139	ug/L	94
21) 2-Butanone	4.735	43		8275	3.039	ug/L	99
22) cis-1,2-Dichloroethene	4.674	96		15680	1.412	ug/L	94
30) Cyclohexane	5.398	56		2315	0.133	ug/L #	81
33) Benzene	5.777	78		48177	1.147	ug/L	100
34) Trichloroethene	6.546	95		70021	6.249	ug/L	95
47) Tetrachloroethene	8.555	164		328563	36.135	ug/L	92
53) m,p-Xylene	9.693	106		1967	0.098	ug/L	93
60) Isopropylbenzene	10.484	105		11541	0.214	ug/L	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
Data File : VU047313.D
Acq On : 03 Mar 2022 14:24
Operator : SY/MD
Sample : N1773-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFY11

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/04/2022
Supervised By :Mahesh Dadoda 03/04/2022

Quant Time: Mar 04 01:55:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 04 01:50:04 2022
Response via : Initial Calibration

