

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
 Data File : VU047314.D
 Acq On : 03 Mar 2022 14:48
 Operator : SY/MD
 Sample : N1773-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1




Instrument :
 MSVOA_U
 ClientSampleId :
 BFY10

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/04/2022
 Supervised By :Mahesh Dadoda 03/04/2022

03/04/2022
 Supervised By :Mahesh
 Dadoda

Quant Time: Mar 04 01:55:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 04 01:50:04 2022
 Response via : Initial Calibration

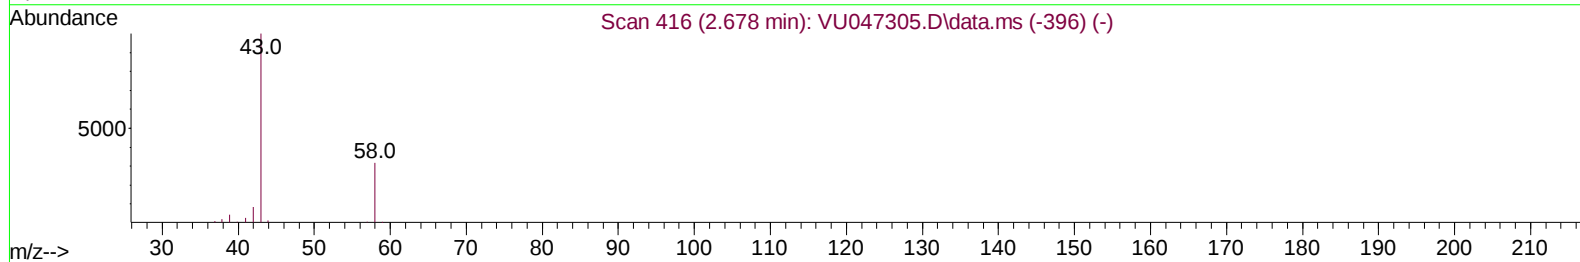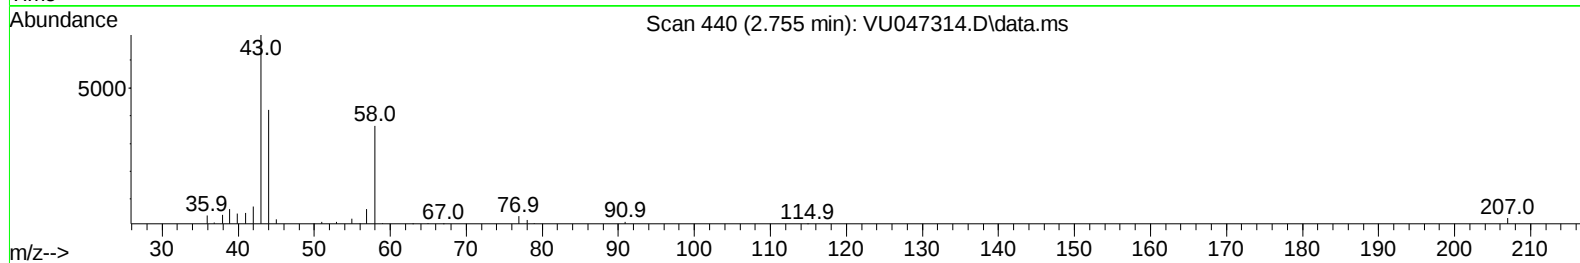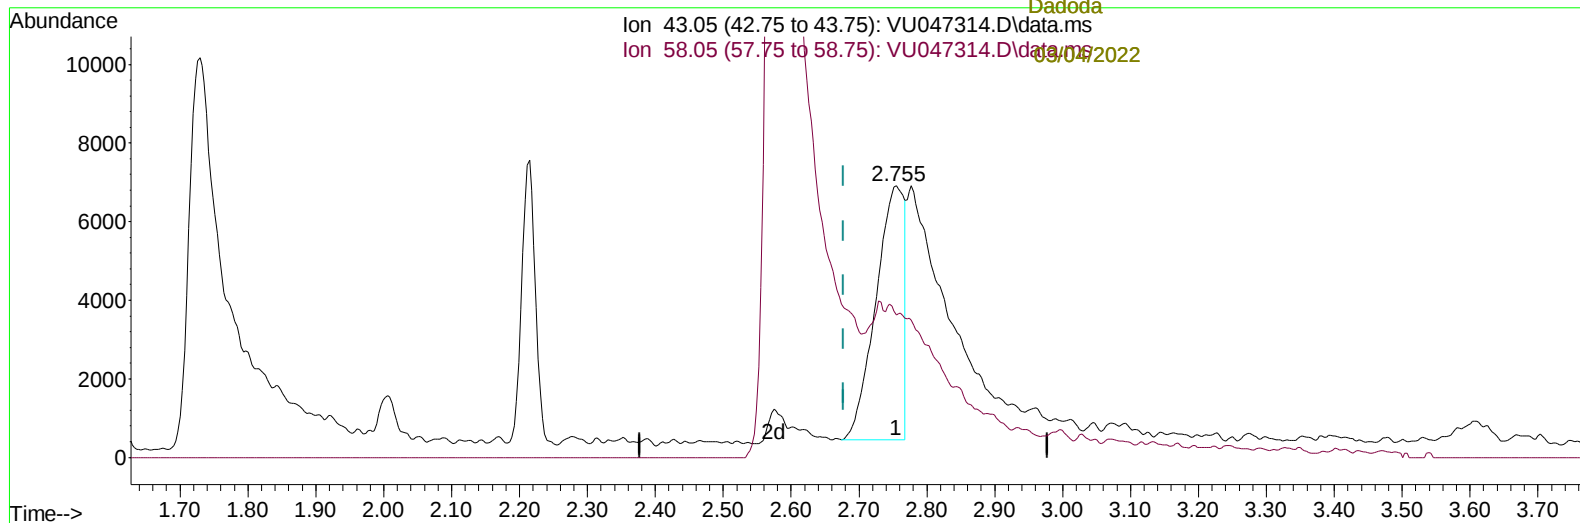

TIC: VU047314.D\data.ms

(13) Acetone (T)

2.755min (+ 0.077) 14.62 ug/L

response 18721

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
 Data File : VU047314.D
 Acq On : 03 Mar 2022 14:48
 Operator : SY/MD
 Sample : N1773-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1




Instrument :
 MSVOA_U
 ClientSampleId :
 BFY10

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/04/2022
 Supervised By :Mahesh Dadoda 03/04/2022

Quant Time: Mar 04 01:55:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 04 01:50:04 2022
 Response via : Initial Calibration

03/04/2022
 Supervised By :Mahesh
 Dadoda
 03/04/2022

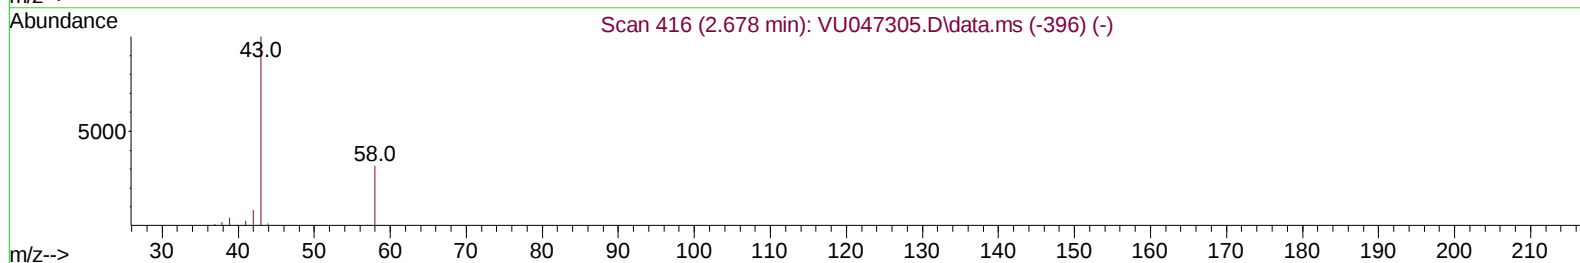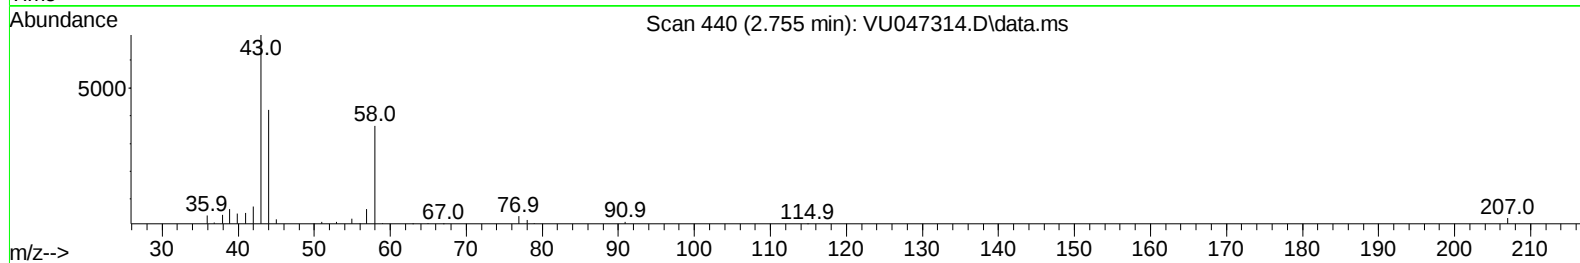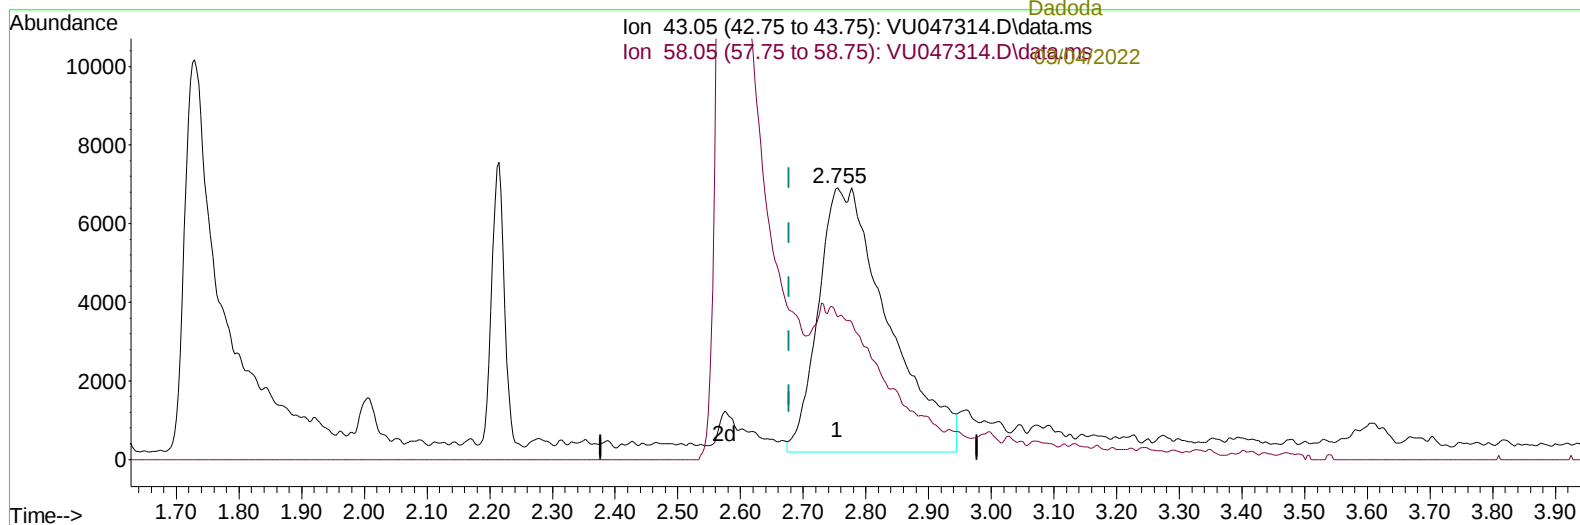

TIC: VU047314.D\data.ms

(13) Acetone (T)

2.755min (+ 0.077) 40.64 ug/L m

response 52029

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	0.00
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
 Data File : VU047314.D
 Acq On : 03 Mar 2022 14:48
 Operator : SY/MD
 Sample : N1773-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFY10

Manual IntegrationsAPPROVED

Reviewed By : John Carlone 03/04/2022
 Supervised By : Mahesh Dadoda 03/04/2022

Quant Time: Mar 04 01:55:21 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 04 01:50:04 2022
 Response via : Initial Calibration

03/04/2022
 Supervised By : Mahesh
 Dadoda

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
-----03/04/2022						
Internal Standards						
1) 1,4-Difluorobenzene	6.276	114	126679	5.000	ug/L	0.02
28) Chlorobenzene-d5	9.423	117	131062	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	80512	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.604	65	45942	4.294	ug/L	0.00
Spiked Amount 5.000	Range 40 - 130		Recovery =	85.800%		
7) Chloroethane-d5	1.925	69	37339	4.404	ug/L	0.00
Spiked Amount 5.000	Range 65 - 130		Recovery =	88.000%		
11) 1,1-Dichloroethene-d2	2.575	65	21324	4.819	ug/L	0.00
Spiked Amount 5.000	Range 60 - 125		Recovery =	96.400%		
20) 2-Butanone-d5	4.732	46	123065	48.124	ug/L	0.08
Spiked Amount 50.000	Range 40 - 130		Recovery =	96.240%		
24) Chloroform-d	5.076	84	78354	4.409	ug/L	0.00
Spiked Amount 5.000	Range 70 - 125		Recovery =	88.200%		
26) 1,2-Dichloroethane-d4	5.729	65	42191	4.269	ug/L	0.02
Spiked Amount 5.000	Range 70 - 130		Recovery =	85.400%		
32) Benzene-d6	5.745	84	153759	4.199	ug/L	0.01
Spiked Amount 5.000	Range 70 - 125		Recovery =	84.000%		
36) 1,2-Dichloropropane-d6	6.716	67	50002	4.291	ug/L	0.02
Spiked Amount 5.000	Range 60 - 140		Recovery =	85.800%		
41) Toluene-d8	7.912	98	142404	3.975	ug/L	0.01
Spiked Amount 5.000	Range 70 - 130		Recovery =	79.600%		
43) trans-1,3-Dichloroprop...	8.195	79	22004	4.166	ug/L	0.01
Spiked Amount 5.000	Range 55 - 130		Recovery =	83.400%		
46) 2-Hexanone-d5	8.655	63	119245	42.874	ug/L	0.02
Spiked Amount 50.000	Range 45 - 130		Recovery =	85.740%		
56) 1,1,2,2-Tetrachloroeth...	10.761	84	47793	4.513	ug/L	0.00
Spiked Amount 5.000	Range 65 - 120		Recovery =	90.200%		
66) 1,2-Dichlorobenzene-d4	12.195	152	62748	4.344	ug/L	0.00
Spiked Amount 5.000	Range 80 - 120		Recovery =	86.800%		
Target Compounds						
					Qvalue	
13) Acetone	2.755	43	52029m	40.641	ug/L	
33) Benzene	5.793	78	4518	0.121	ug/L	100
47) Tetrachloroethene	8.562	164	2466	0.306	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
Data File : VU047314.D
Acq On : 03 Mar 2022 14:48
Operator : SY/MD
Sample : N1773-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFY10

Manual IntegrationsAPPROVED

Reviewed By :John Carlone 03/04/2022
Supervised By :Mahesh Dadoda 03/04/2022

03/04/2022
Supervised By :Mahesh
Dadoda

03/04/2022

Quant Time: Mar 04 01:55:21 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 04 01:50:04 2022
Response via : Initial Calibration

