

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
 Data File : VU047306.D
 Acq On : 03 Mar 2022 10:27
 Operator : SY/MD
 Sample : VU0303WBL01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VBLK070

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047306.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.600	74	81	93	rBV	60165	70099	12.20%	1.606%
2	1.919	171	180	200	rBV	49430	68244	11.87%	1.564%
3	2.571	372	383	397	rVB	106526	171860	29.90%	3.938%
4	3.051	522	532	549	rVB4	8876	17275	3.01%	0.396%
5	4.655	1013	1031	1074	rBV	49201	226242	39.36%	5.184%
6	5.067	1144	1159	1185	rVB2	88357	196383	34.17%	4.500%
7	5.729	1343	1365	1384	rBV2	181479	465443	80.98%	10.665%
8	6.253	1513	1528	1552	rBV	160792	305018	53.07%	6.989%
9	6.693	1645	1665	1683	rBV	110699	215924	37.57%	4.948%
10	7.568	1924	1937	1952	rBV	64040	110225	19.18%	2.526%
11	7.899	2026	2040	2058	rBV	232093	399216	69.45%	9.148%
12	8.182	2116	2128	2143	rBV2	40394	71202	12.39%	1.632%
13	8.475	2207	2219	2229	rBV2	4451	8167	1.42%	0.187%
14	8.639	2256	2270	2301	rBV	306701	574786	100.00%	13.171%
15	9.417	2499	2512	2534	rBV	240253	398615	69.35%	9.134%
16	10.758	2917	2929	2948	rVB	103380	165745	28.84%	3.798%
17	10.893	2963	2971	2983	rVB2	4039	6472	1.13%	0.148%
18	11.812	3243	3257	3274	rBV	310423	488946	85.07%	11.204%
19	12.192	3362	3375	3394	rBV	246474	404187	70.32%	9.262%




Sum of corrected areas: 4364049

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
Data File : VU047306.D
Acq On : 03 Mar 2022 10:27
Operator : SY/MD
Sample : VU0303WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK070

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

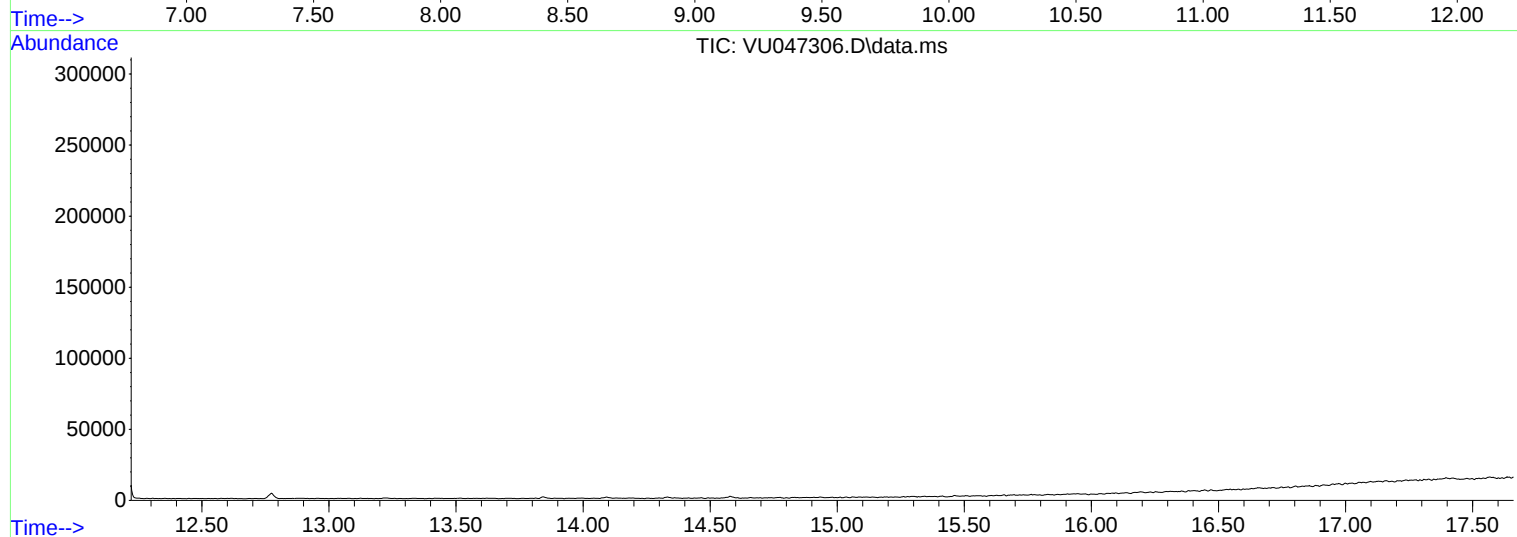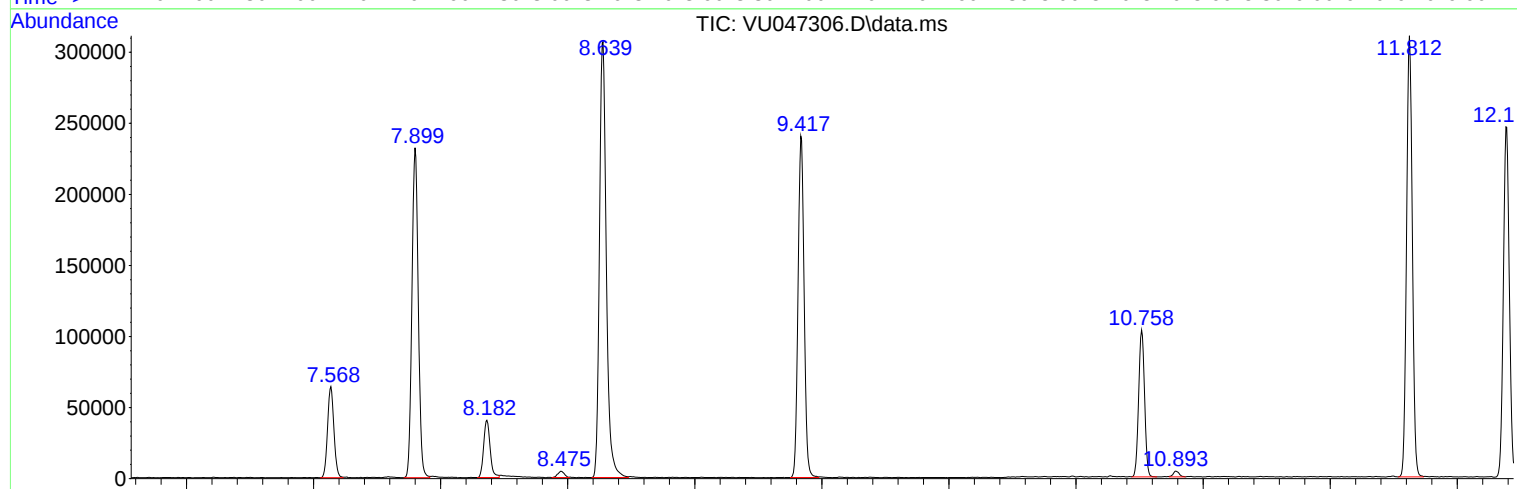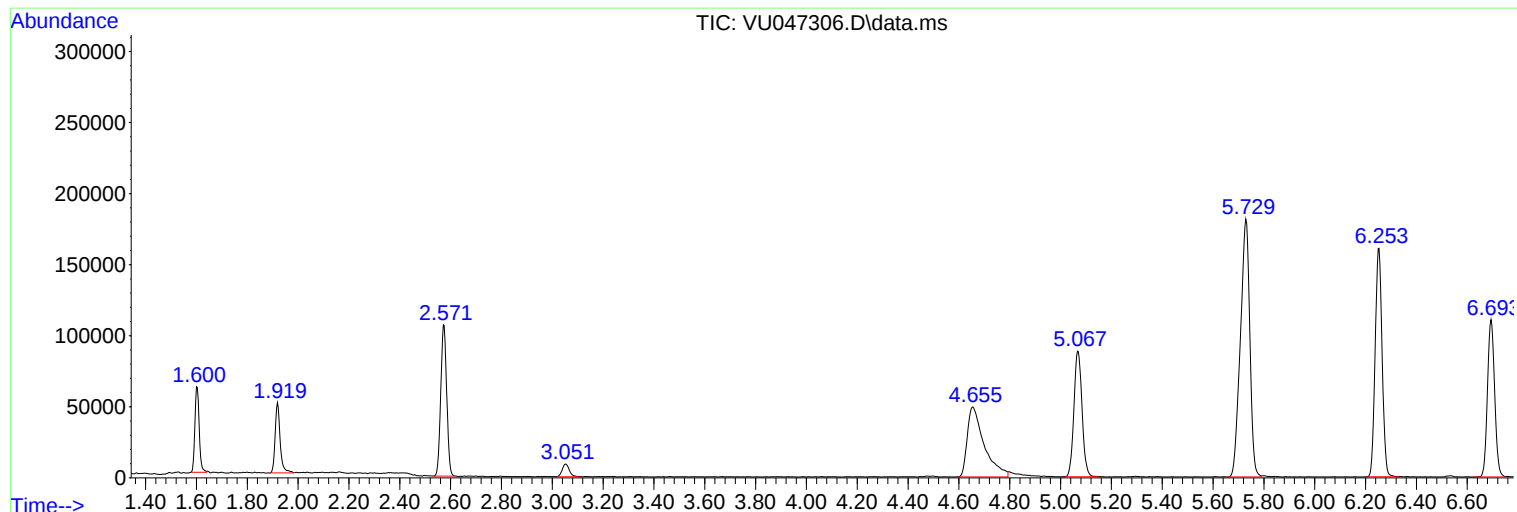

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
Data File : VU047306.D
Acq On : 03 Mar 2022 10:27
Operator : SY/MD
Sample : VU0303WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK070

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
Data File : VU047306.D
Acq On : 03 Mar 2022 10:27
Operator : SY/MD
Sample : VU0303WBL01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VBLK070

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc