

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
 Data File : VU047315.D
 Acq On : 03 Mar 2022 15:12
 Operator : SY/MD
 Sample : VIBLK007
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VIBLK007

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU047315.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	96	rBV	59936	69517	12.16%	1.557%
2	1.919	172	180	199	rBV	47475	63756	11.15%	1.428%
3	2.572	372	383	398	rVB	103783	167935	29.38%	3.761%
4	3.051	522	532	546	rBV	7279	13413	2.35%	0.300%
5	4.652	1013	1030	1086	rBV	50818	239911	41.98%	5.373%
6	5.067	1143	1159	1180	rBV	88552	195005	34.12%	4.367%
7	5.729	1343	1365	1389	rBV2	177053	458774	80.27%	10.275%
8	6.250	1513	1527	1544	rBV	157975	300063	52.50%	6.720%
9	6.694	1651	1665	1683	rBV	111246	215082	37.63%	4.817%
10	7.568	1924	1937	1955	rBV	61358	109525	19.16%	2.453%
11	7.899	2026	2040	2057	rBV	226900	389965	68.23%	8.734%
12	8.182	2116	2128	2142	rBV	39941	68489	11.98%	1.534%
13	8.475	2207	2219	2232	rBV2	7816	18629	3.26%	0.417%
14	8.636	2256	2269	2308	rBV	292412	571547	100.00%	12.801%
15	8.787	2308	2316	2328	rVB3	8876	14861	2.60%	0.333%
16	9.417	2500	2512	2536	rBV	240234	399552	69.91%	8.949%
17	10.758	2918	2929	2945	rVB2	104785	166468	29.13%	3.728%
18	10.896	2961	2972	2988	rVB2	14286	26505	4.64%	0.594%
19	11.687	3211	3218	3227	rVB4	4395	6212	1.09%	0.139%
20	11.812	3244	3257	3274	rBV	311032	487541	85.30%	10.919%
21	12.192	3362	3375	3393	rBV	248942	397647	69.57%	8.906%
22	12.774	3545	3556	3570	rBV2	9562	15999	2.80%	0.358%
23	12.890	3583	3592	3602	rVB4	9790	15245	2.67%	0.341%
24	14.735	4157	4166	4175	rBV6	6845	9915	1.73%	0.222%
25	16.886	4827	4835	4845	rVB	30096	43413	7.60%	0.972%




Sum of corrected areas: 4464969

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
Data File : VU047315.D
Acq On : 03 Mar 2022 15:12
Operator : SY/MD
Sample : VIBLK007
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK007

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

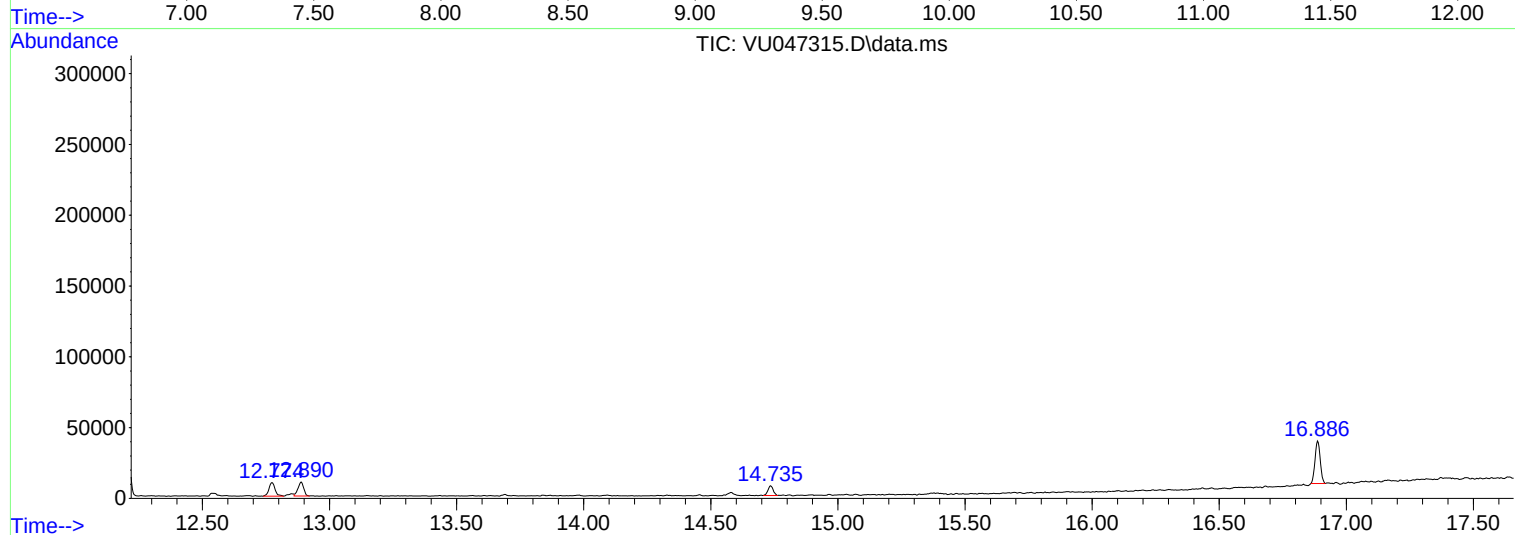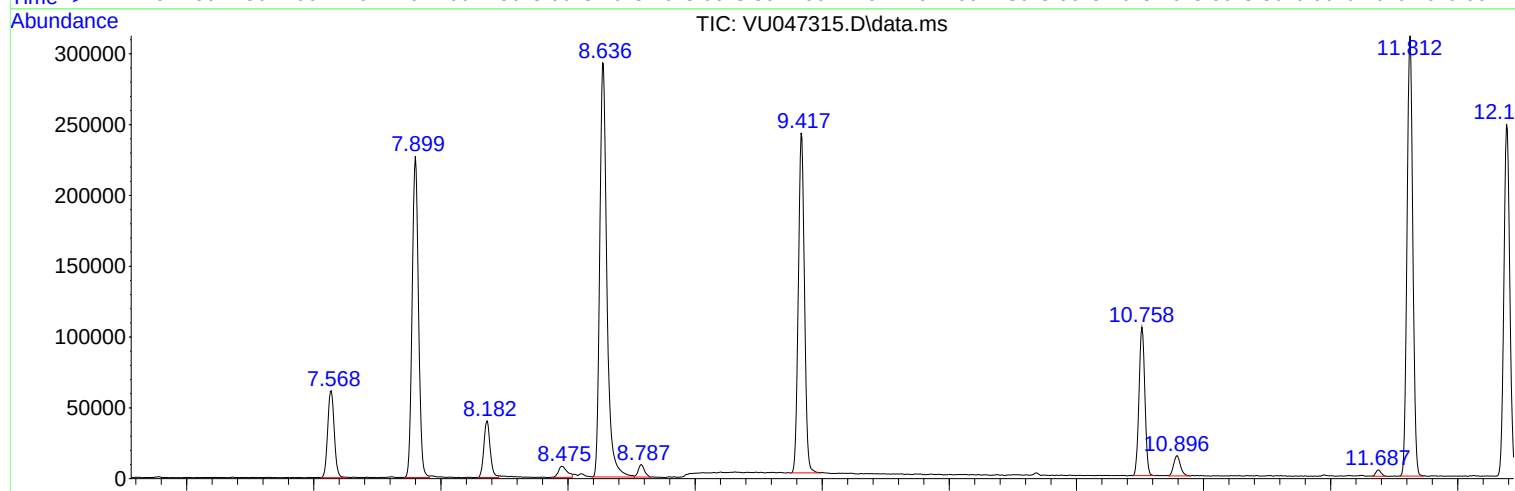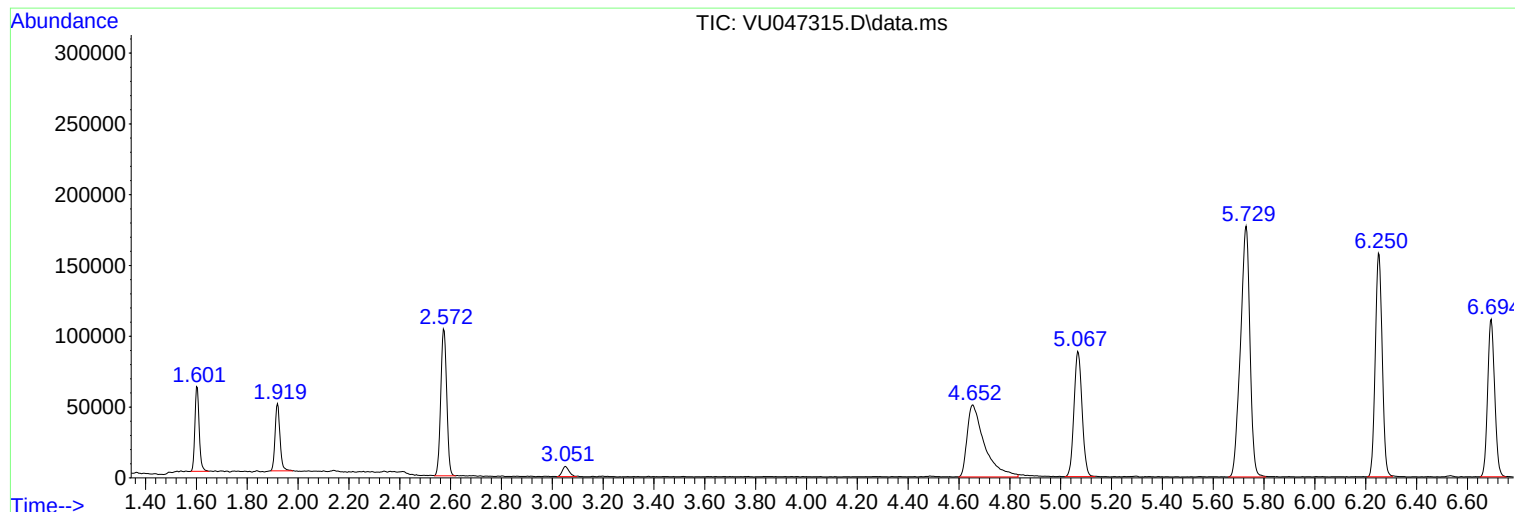

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
Data File : VU047315.D
Acq On : 03 Mar 2022 15:12
Operator : SY/MD
Sample : VIBLK007
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK007

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
Data File : VU047315.D
Acq On : 03 Mar 2022 15:12
Operator : SY/MD
Sample : VIBLK007
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VIBLK007

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc