

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
 Data File : VU047320.D
 Acq On : 03 Mar 2022 17:10
 Operator : SY/MD
 Sample : N1775-09
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 DBRX2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047320.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	96	rVB	55912	65160	11.75%	1.549%
2	1.919	172	180	192	rBV	45348	60763	10.95%	1.445%
3	2.572	372	383	398	rVB	99167	159768	28.80%	3.798%
4	4.652	1013	1030	1077	rBV	51777	228619	41.21%	5.435%
5	5.067	1144	1159	1184	rBV	85117	189808	34.21%	4.513%
6	5.729	1343	1365	1392	rBV2	170422	439334	79.19%	10.445%
7	6.250	1514	1527	1552	rBV	158497	299784	54.04%	7.127%
8	6.694	1651	1665	1683	rBV	105085	204244	36.82%	4.856%
9	7.568	1925	1937	1951	rBV	57863	101766	18.34%	2.419%
10	7.899	2027	2040	2057	rBV	217303	370849	66.85%	8.817%
11	8.182	2117	2128	2141	rBV	37315	63267	11.40%	1.504%
12	8.472	2208	2218	2227	rBV2	3441	6392	1.15%	0.152%
13	8.636	2256	2269	2301	rBV	303445	554777	100.00%	13.190%
14	9.417	2500	2512	2536	rBV	237940	394236	71.06%	9.373%
15	10.758	2917	2929	2946	rBV	100654	160590	28.95%	3.818%
16	10.896	2961	2972	2984	rVB	9784	16184	2.92%	0.385%
17	11.812	3244	3257	3276	rBV	304660	479806	86.49%	11.407%
18	12.060	3326	3334	3351	rBV3	12481	22327	4.02%	0.531%
19	12.192	3363	3375	3392	rVB	238128	382332	68.92%	9.090%
20	12.774	3545	3556	3567	rBV3	3622	6170	1.11%	0.147%




Sum of corrected areas: 4206176

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
Data File : VU047320.D
Acq On : 03 Mar 2022 17:10
Operator : SY/MD
Sample : N1775-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBRX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

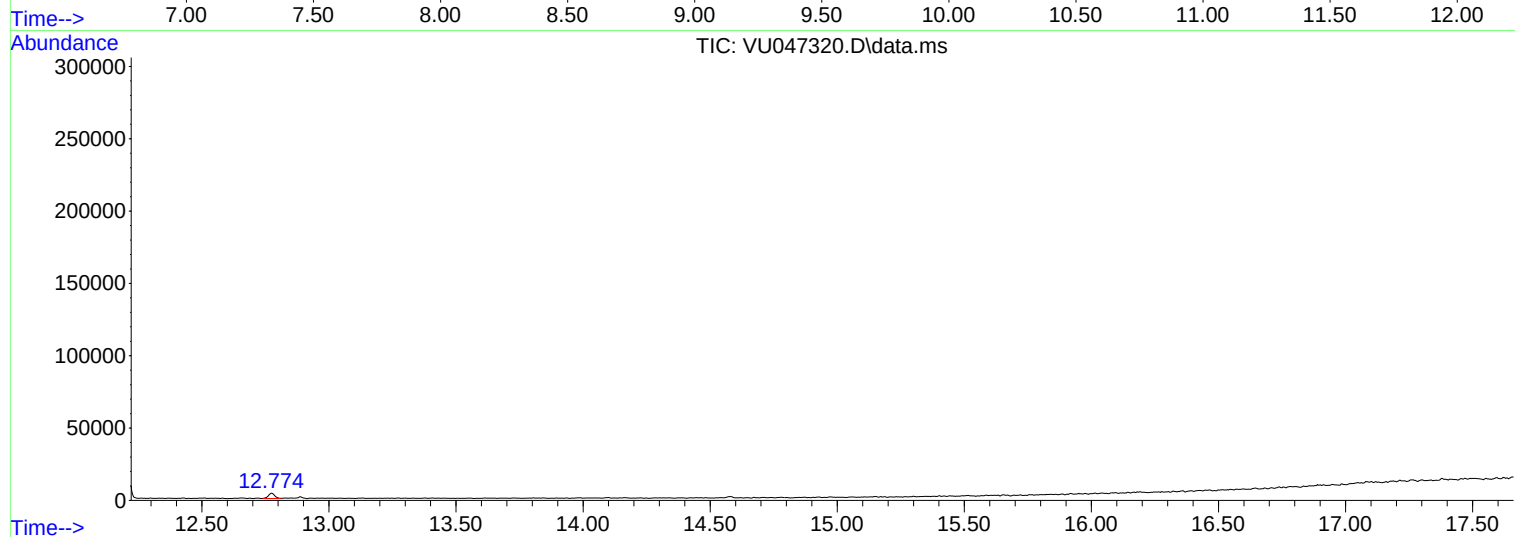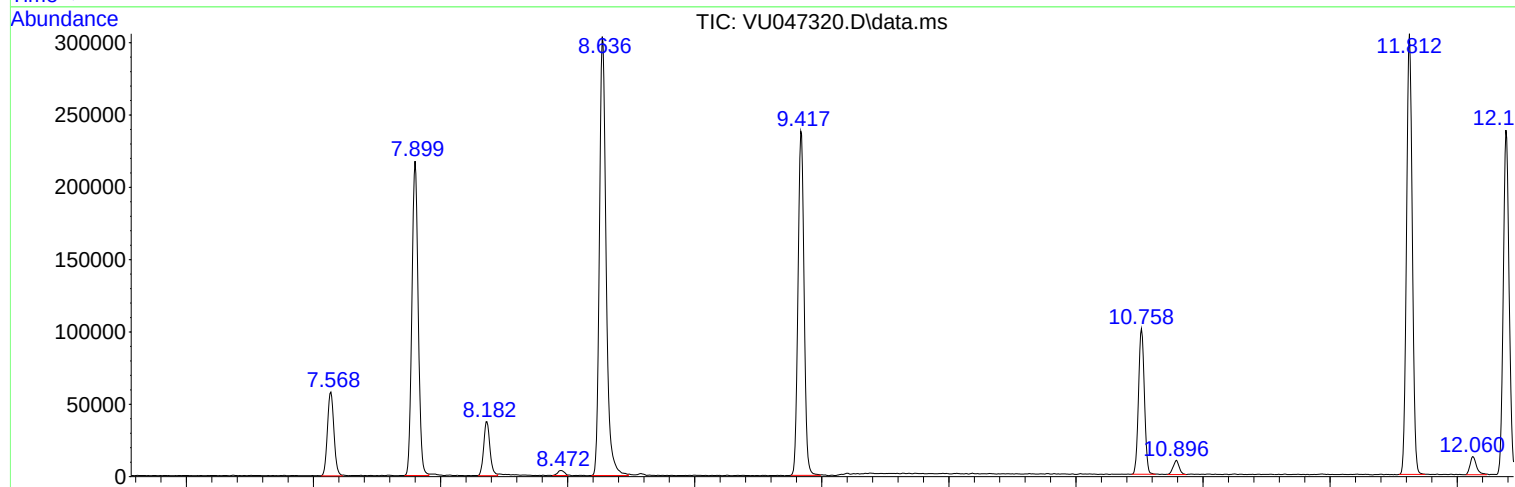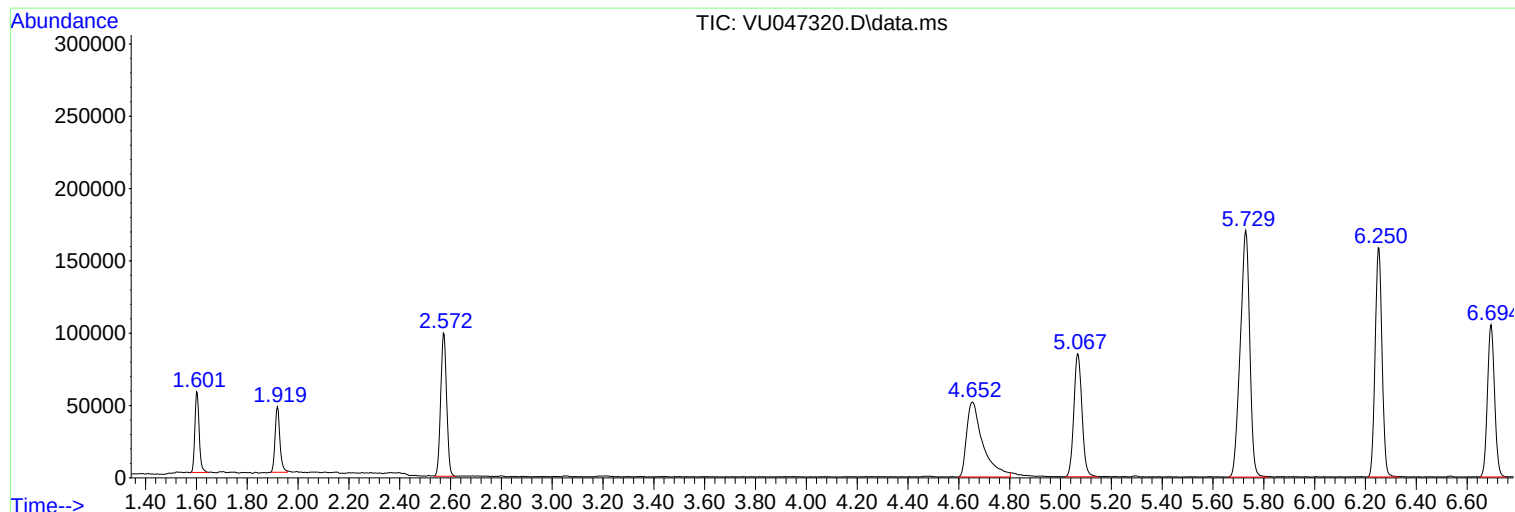

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
Data File : VU047320.D
Acq On : 03 Mar 2022 17:10
Operator : SY/MD
Sample : N1775-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBRX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
Data File : VU047320.D
Acq On : 03 Mar 2022 17:10
Operator : SY/MD
Sample : N1775-09
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
DBRX2

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc