

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
 Data File : VU047321.D
 Acq On : 03 Mar 2022 17:33
 Operator : SY/MD
 Sample : N1775-10
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047321.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	96	rVB	57768	65865	11.85%	1.566%
2	1.919	171	180	197	rBV	46376	61817	11.12%	1.470%
3	2.572	372	383	400	rBV	97705	158945	28.60%	3.779%
4	3.051	523	532	548	rBV2	4576	8570	1.54%	0.204%
5	4.652	1013	1030	1081	rBV2	50843	225704	40.62%	5.366%
6	5.067	1141	1159	1184	rBV	86375	186588	33.58%	4.436%
7	5.729	1343	1365	1383	rBV2	168314	438176	78.85%	10.417%
8	6.250	1514	1527	1555	rVB	155057	293309	52.78%	6.973%
9	6.694	1652	1665	1684	rBV	105253	204407	36.79%	4.860%
10	7.568	1924	1937	1955	rBV	58699	102754	18.49%	2.443%
11	7.899	2027	2040	2058	rBV	220034	375474	67.57%	8.927%
12	8.182	2116	2128	2143	rBV	36993	64163	11.55%	1.525%
13	8.475	2202	2219	2236	rBV2	10527	18926	3.41%	0.450%
14	8.636	2256	2269	2298	rBV	301149	555677	100.00%	13.211%
15	9.417	2500	2512	2543	rVB	232391	388892	69.99%	9.246%
16	10.758	2917	2929	2943	rBV	101682	161592	29.08%	3.842%
17	10.893	2959	2971	2984	rBV	17999	30507	5.49%	0.725%
18	11.812	3245	3257	3272	rBV	301832	471881	84.92%	11.219%
19	12.192	3363	3375	3389	rBV	236326	381138	68.59%	9.061%
20	12.774	3545	3556	3566	rVB	7293	11834	2.13%	0.281%




Sum of corrected areas: 4206219

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
Data File : VU047321.D
Acq On : 03 Mar 2022 17:33
Operator : SY/MD
Sample : N1775-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

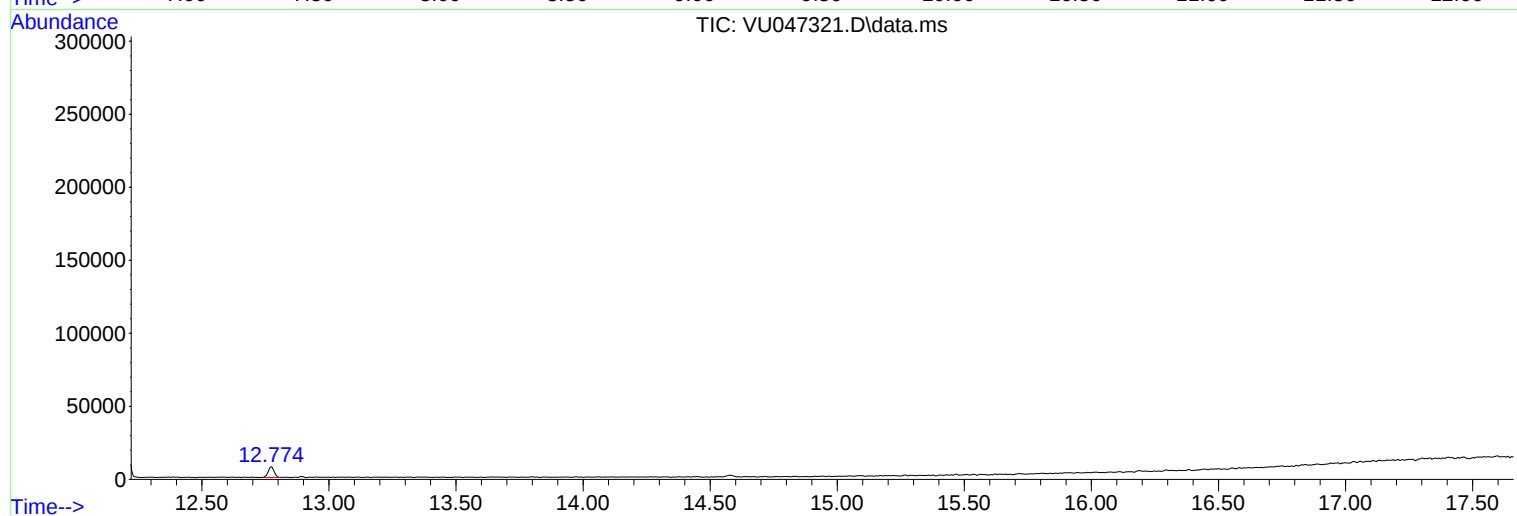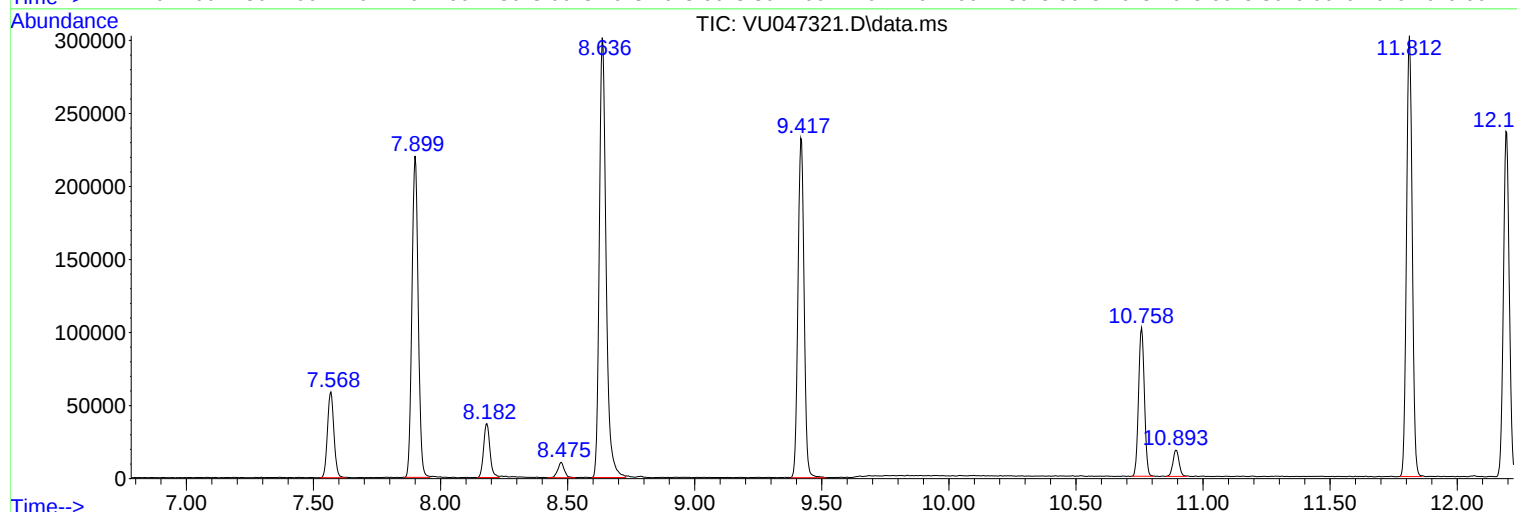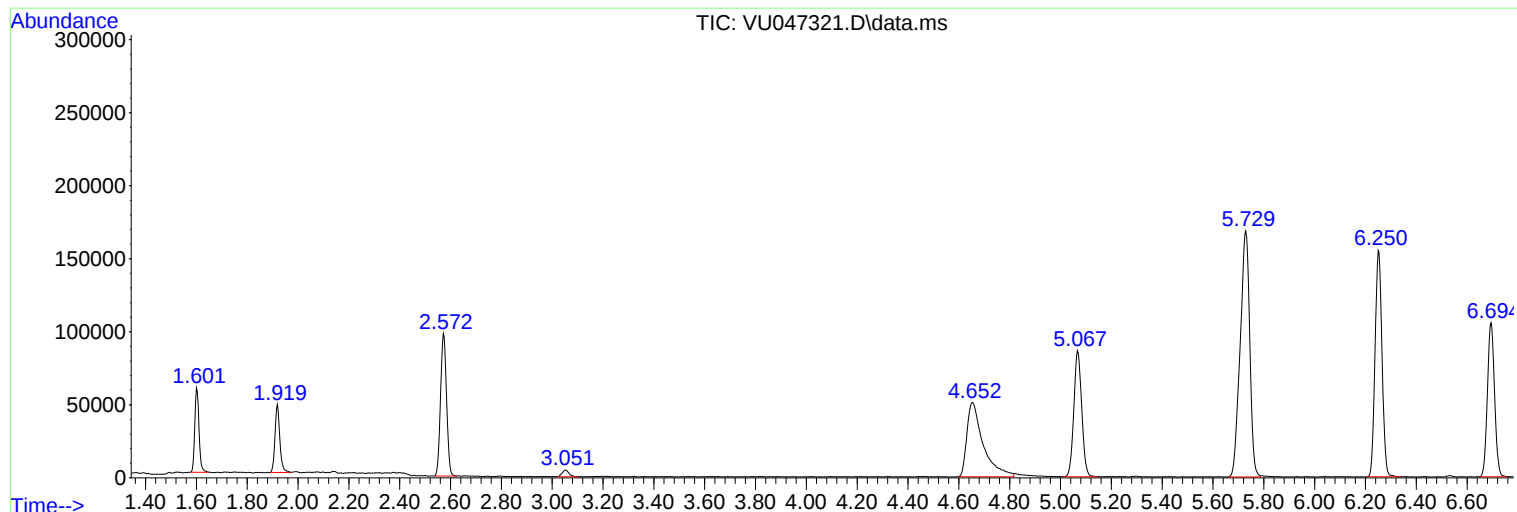

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
Data File : VU047321.D
Acq On : 03 Mar 2022 17:33
Operator : SY/MD
Sample : N1775-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
Data File : VU047321.D
Acq On : 03 Mar 2022 17:33
Operator : SY/MD
Sample : N1775-10
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc