


Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030322\
Data File : VU047304.D
Acq On : 03 Mar 2022 09:02
Operator : SY/MD
Sample : BFB060
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFB060

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR021622WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Fri Mar 04 01:50:04 2022

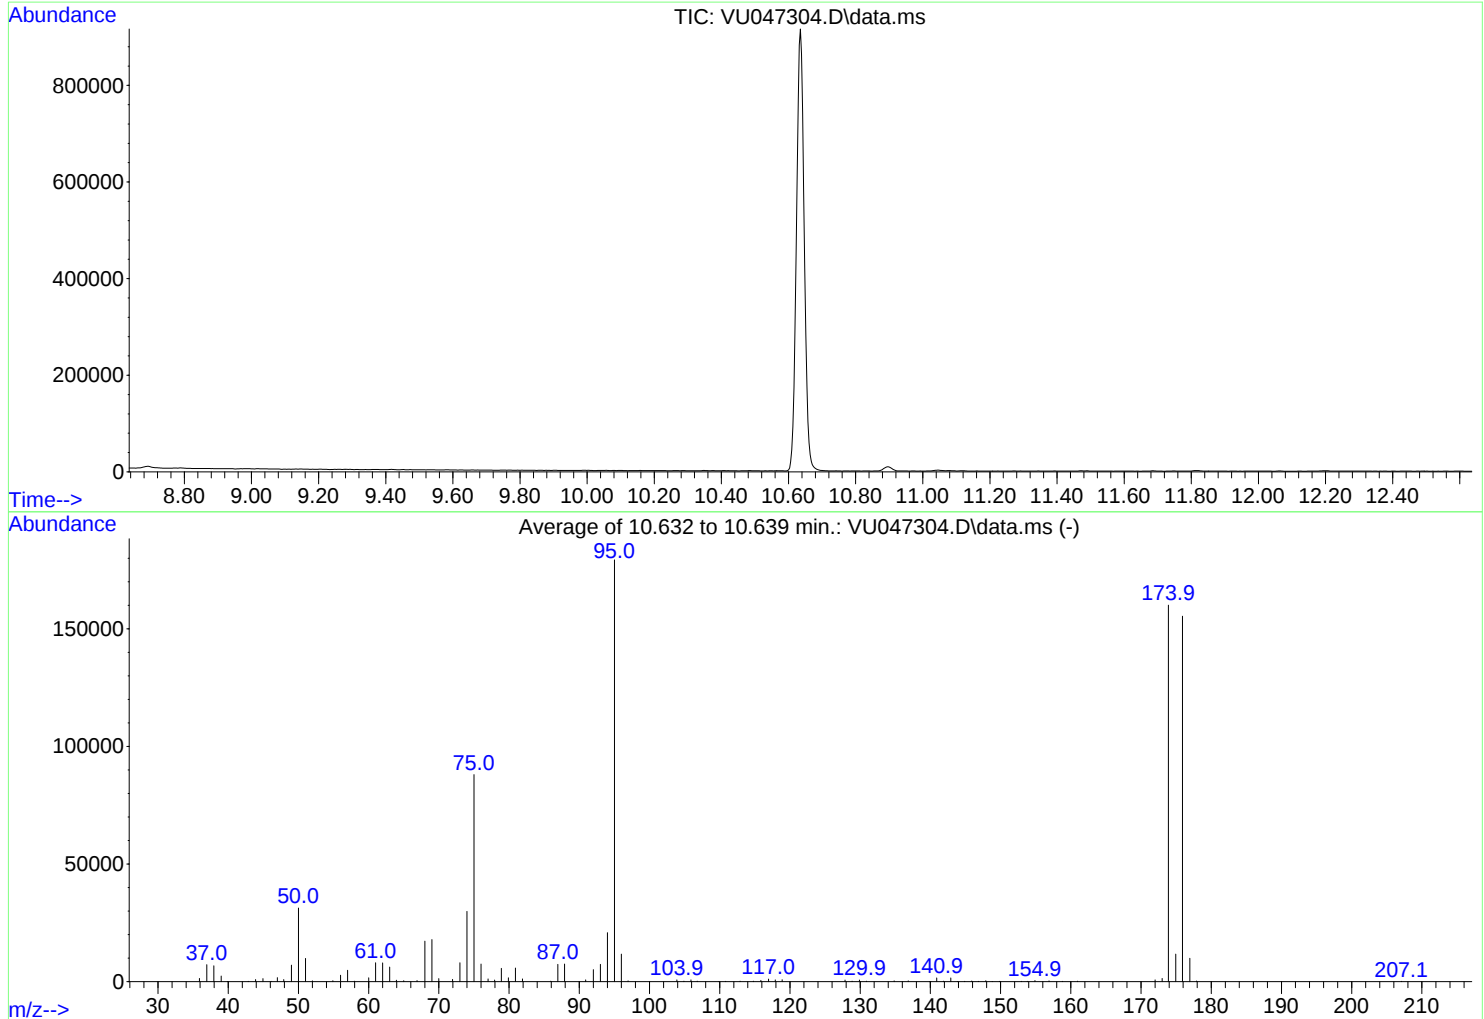

AutoFind: Scans 2890, 2891, 2892; Background Corrected with Scan 2876

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	31280	PASS
75	95	30	80	49.1	88027	PASS
95	95	100	100	100.0	179307	PASS
96	95	5	9	6.5	11725	PASS
173	174	0.00	2	0.8	1352	PASS
174	95	50	120	89.3	160085	PASS
175	174	5	9	7.3	11675	PASS
176	174	95	101	97.0	155328	PASS
177	176	5	9	6.4	9941	PASS

m/z	Abundance
35.90	1058.0
36.80	111.0
37.90	358.0
39.90	244.0
43.90	363.0

Instrument :
MSVOA_U
ClientSampleId :
BFB060

m/z	Abundance
35.90	2432.0
37.00	7477.0
38.00	7284.0
39.00	2528.0
40.00	327.0
42.90	103.0
43.90	1283.0
45.00	1333.0
46.10	136.0
47.00	1676.0
47.90	984.0
49.00	7128.0
50.00	31864.0
51.00	10049.0
52.00	354.0
54.90	429.0
56.00	2627.0
57.00	4629.0
58.00	176.0
60.00	1672.0
61.00	8305.0
62.00	8100.0
63.00	6377.0
63.90	610.0
65.00	453.0
66.90	474.0
68.00	17568.0
69.00	18176.0
70.00	1398.0
71.90	1072.0
73.00	8054.0
74.00	29888.0
75.00	88864.0
76.00	7739.0
77.00	1171.0
78.00	709.0
78.90	5554.0
79.90	1670.0
80.90	5742.0
81.90	1126.0
85.90	177.0
86.90	7414.0
87.90	7652.0
90.90	735.0
92.00	5102.0
93.00	7551.0
94.00	20584.0
95.00	178816.0
96.00	11902.0
96.90	335.0
103.90	726.0
104.90	211.0
105.90	723.0
106.80	192.0
109.90	130.0
110.80	170.0
112.90	186.0
114.80	171.0
115.90	481.0
116.90	1075.0
117.90	732.0
118.90	810.0
127.80	639.0
128.90	250.0
129.90	704.0
130.90	257.0
134.90	312.0
136.90	297.0
139.90	112.0
140.90	1600.0
141.90	238.0
142.90	1511.0
143.90	103.0
144.90	157.0
145.90	285.0
146.90	109.0
147.90	420.0
149.90	121.0
153.00	120.0
153.80	164.0
154.90	442.0
156.90	287.0
158.80	163.0
160.90	176.0
172.00	808.0
173.00	1330.0
173.90	156672.0
174.90	11546.0
175.90	150912.0
176.90	9706.0
177.90	289.0
207.10	132.0

Instrument :
MSVOA_U
ClientSampleId :
BFB060

m/z	Abundance
36.00	2460.0
37.00	7550.0
38.00	7214.0
39.00	2460.0
40.00	327.0
42.80	133.0
44.00	1235.0
45.00	1354.0
46.10	157.0
47.00	1764.0
47.90	936.0
49.00	7244.0
50.00	32176.0
51.00	10263.0
52.00	368.0
54.90	432.0
56.00	2802.0
57.00	5043.0
57.90	186.0
60.00	1687.0
61.00	8260.0
62.00	8148.0
63.00	6413.0
64.00	616.0
65.00	417.0
66.90	480.0
68.00	17656.0
69.00	18496.0
70.00	1360.0
72.00	986.0
73.00	8335.0
74.00	30808.0
75.00	90864.0
76.00	7733.0
77.00	1185.0
78.00	735.0
78.90	5752.0
79.90	1661.0
80.90	5933.0
81.90	1198.0
85.90	186.0
87.00	7586.0
87.90	7764.0
90.90	780.0
92.00	5220.0
93.00	7623.0
94.00	21536.0
95.00	185216.0
96.00	12063.0
97.00	330.0
103.90	768.0
104.90	210.0
105.90	765.0
106.80	204.0
109.90	122.0
110.90	172.0
112.90	196.0
114.80	207.0
115.80	557.0
116.90	1124.0
117.90	774.0
118.90	870.0
127.90	682.0
128.90	237.0
129.90	741.0
130.90	246.0
134.80	335.0
136.90	345.0
140.10	106.0
140.90	1646.0
141.80	209.0
142.90	1601.0
143.80	100.0
144.90	184.0
145.90	282.0
146.90	125.0
147.90	449.0
148.80	116.0
149.80	167.0
152.90	131.0
153.80	150.0
154.90	464.0
156.90	343.0
158.80	160.0
160.90	190.0
172.00	823.0
173.00	1408.0
173.90	165376.0
175.00	12073.0
175.90	160128.0
176.90	10234.0
177.90	295.0

Instrument :
MSVOA_U
ClientSampleId :
BFB060

207.10

133.0

Instrument :
MSVOA_U
ClientSampleId :
BFB060

m/z	Abundance
36.00	2376.0
37.00	7021.0
38.00	6724.0
39.00	2231.0
39.90	308.0
42.90	132.0
44.00	1152.0
44.90	1311.0
46.10	155.0
47.00	1651.0
47.90	850.0
49.00	6722.0
50.00	29800.0
51.00	9265.0
52.00	352.0
54.90	412.0
56.00	2723.0
57.00	4834.0
57.90	174.0
60.00	1502.0
61.00	7560.0
62.00	7629.0
63.00	5877.0
64.00	542.0
65.00	378.0
66.90	442.0
68.00	16335.0
69.00	17024.0
70.00	1241.0
72.00	857.0
73.00	7772.0
74.00	28904.0
75.00	84352.0
76.00	6990.0
77.00	1097.0
77.90	712.0
78.90	5541.0
79.90	1515.0
80.90	5582.0
81.90	1184.0
86.00	199.0
87.00	7081.0
87.90	6986.0
90.90	724.0
92.00	4945.0
93.00	6879.0
94.00	20280.0
95.00	173888.0
96.00	11210.0
97.00	298.0
103.90	755.0
104.90	203.0
105.90	726.0
106.80	181.0
110.90	151.0
112.90	166.0
114.80	219.0
115.80	560.0
117.00	1024.0
117.90	681.0
118.90	831.0
127.90	672.0
128.80	210.0
129.90	652.0
130.90	217.0
134.80	291.0
136.80	320.0
140.00	114.0
140.90	1512.0
141.80	174.0
142.90	1577.0
144.90	183.0
145.90	242.0
146.80	122.0
147.90	438.0
148.80	121.0
149.80	185.0
152.90	129.0
153.80	130.0
154.90	461.0
156.90	377.0
158.80	160.0
161.00	193.0
172.00	723.0
173.00	1317.0
173.90	158208.0
175.00	11405.0
175.90	154944.0
177.00	9883.0
177.90	253.0
207.10	108.0

Instrument :
MSVOA_U
ClientSampleId :
BFB060