




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030422\
 Data File : VU047334.D
 Acq On : 04 Mar 2022 17:07
 Operator : SY/MD
 Sample : N1773-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFY14

Manual IntegrationsAPPROVED

Quant Time: Mar 04 23:23:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 04 23:20:39 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/07/2022
 Supervised By :Mahesh Dadoda 03/07/2022

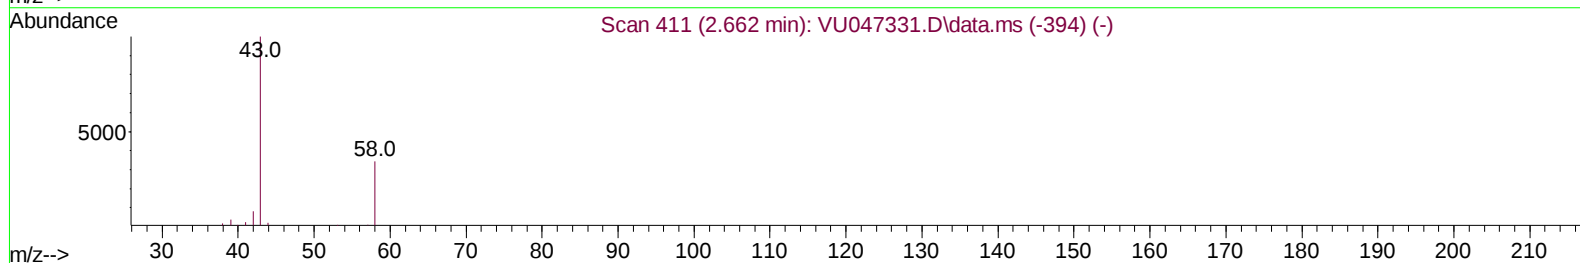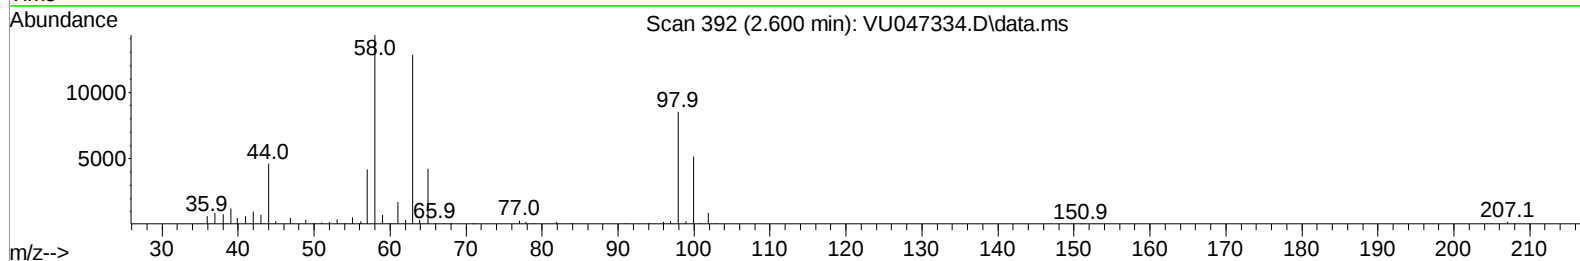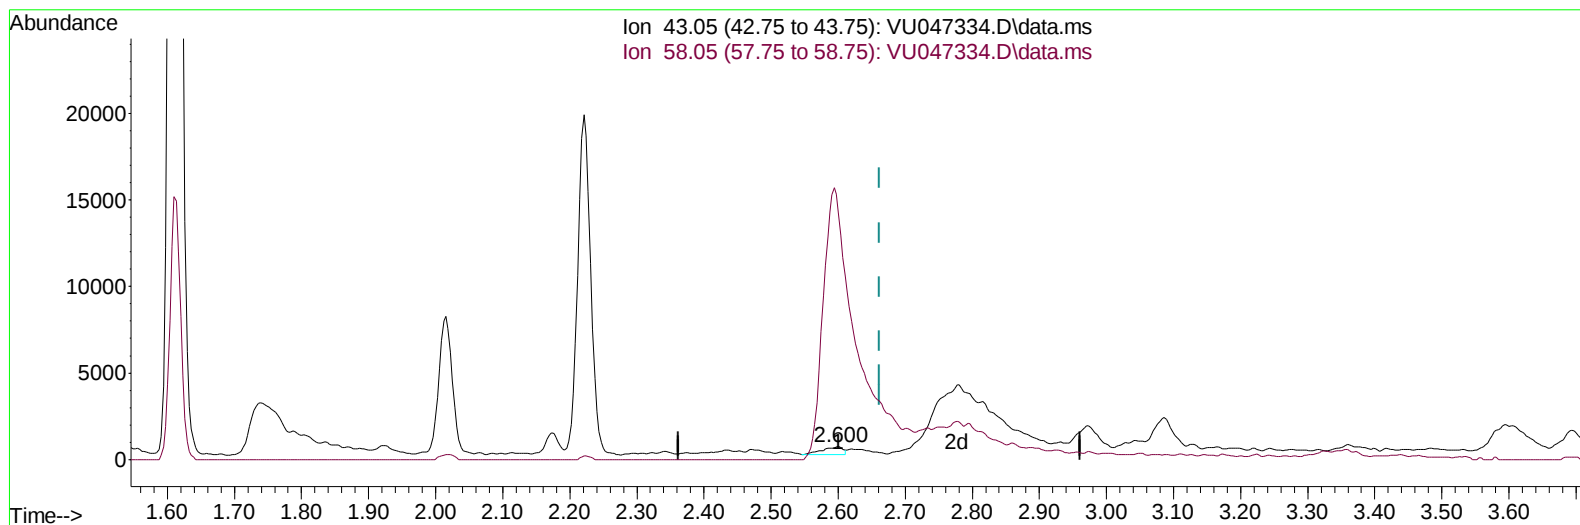

TIC: VU047334.D\data.ms

(13) Acetone (T)

2.600min (-0.061) 0.49 ug/L

response 944

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	5722.56#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030422\
 Data File : VU047334.D
 Acq On : 04 Mar 2022 17:07
 Operator : SY/MD
 Sample : N1773-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFY14

Manual IntegrationsAPPROVED

Quant Time: Mar 04 23:23:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 04 23:20:39 2022
 Response via : Initial Calibration

Reviewed By :John Carlone 03/07/2022
 Supervised By :Mahesh Dadoda 03/07/2022

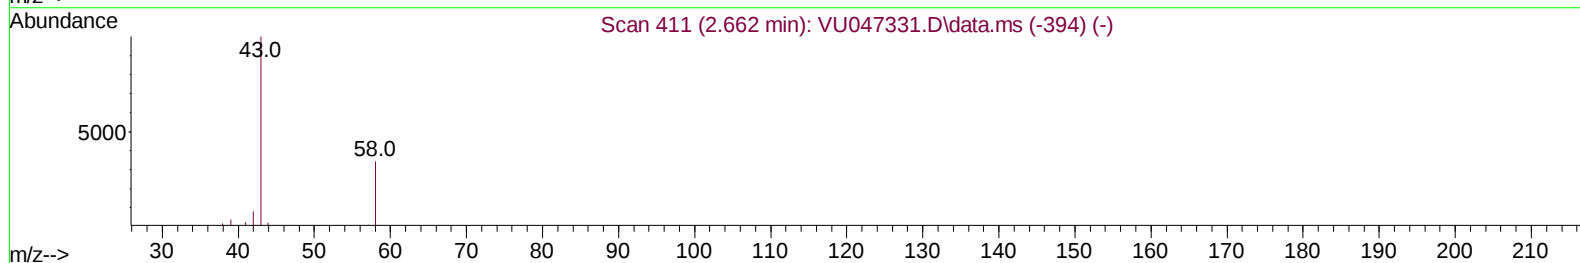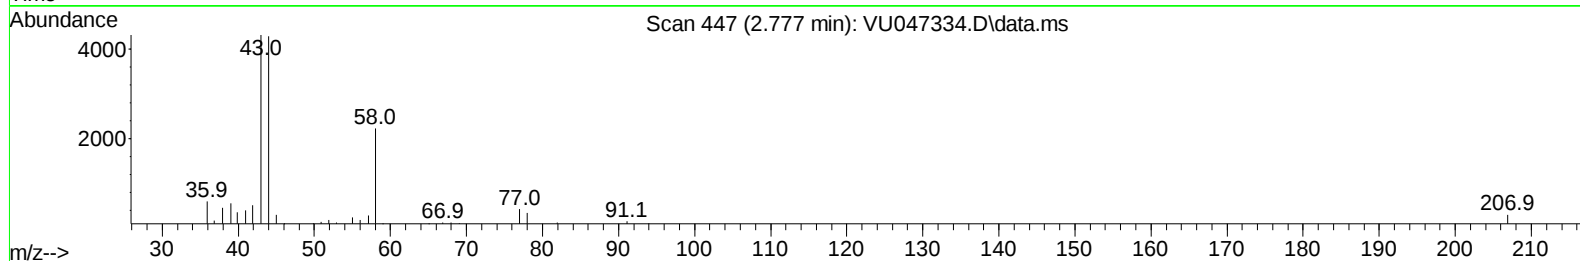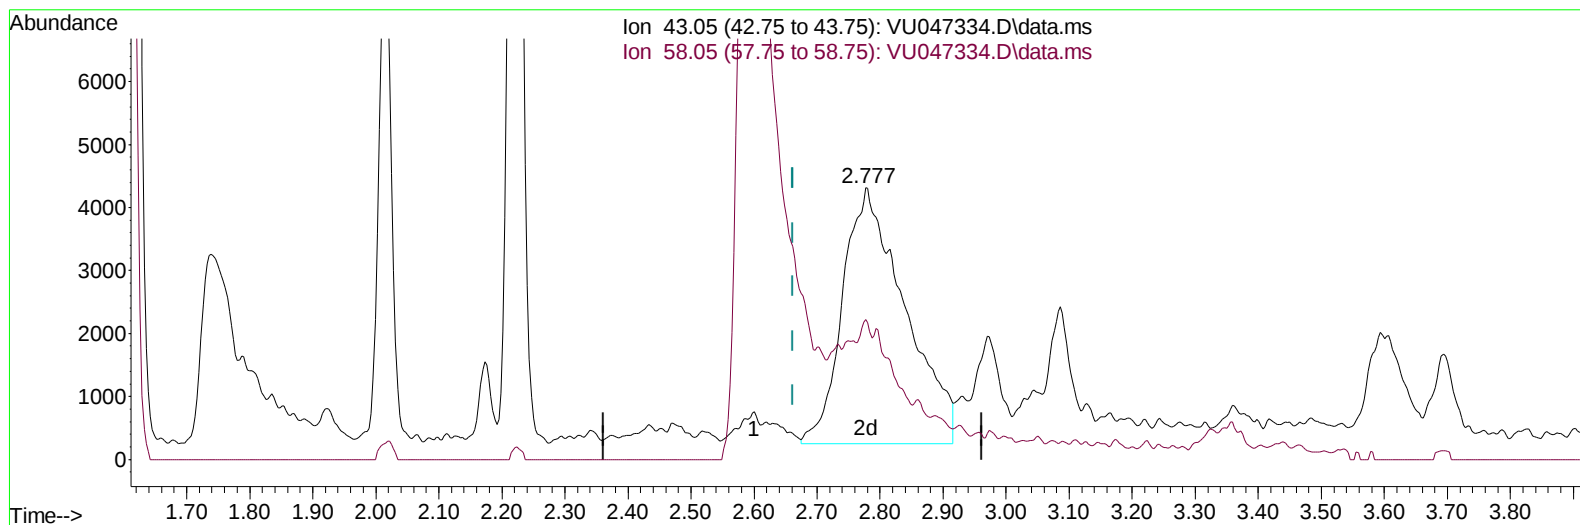

TIC: VU047334.D\data.ms

(13) Acetone (T)

2.777min (+ 0.116) 14.44 ug/L m

response 27785

Ion	Exp%	Act%
43.05	100.00	100.00
58.05	35.80	194.43#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030422\
 Data File : VU047334.D
 Acq On : 04 Mar 2022 17:07
 Operator : SY/MD
 Sample : N1773-07
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFY14

Manual IntegrationsAPPROVED

Quant Time: Mar 04 23:23:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 04 23:20:39 2022
 Response via : Initial Calibration

Reviewed By : John Carlone 03/07/2022
 Supervised By : Mahesh Dadoda 03/07/2022

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	6.282	114	204513	5.000	ug/L	0.03
28) Chlorobenzene-d5	9.427	117	199992	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	114054	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.610	65	63833	4.398	ug/L	0.00
Spiked Amount 5.000	Range 40	- 130	Recovery	=	88.000%	
7) Chloroethane-d5	1.935	69	55521	4.585	ug/L	0.02
Spiked Amount 5.000	Range 65	- 130	Recovery	=	91.800%	
11) 1,1-Dichloroethene-d2	2.584	65	28880	4.711	ug/L	0.00
Spiked Amount 5.000	Range 60	- 125	Recovery	=	94.200%	
20) 2-Butanone-d5	4.742	46	174284	36.574	ug/L	0.10
Spiked Amount 50.000	Range 40	- 130	Recovery	=	73.140%	
24) Chloroform-d	5.079	84	109547	4.085	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	81.600%	
26) 1,2-Dichloroethane-d4	5.729	65	61450	4.083	ug/L	0.02
Spiked Amount 5.000	Range 70	- 130	Recovery	=	81.600%	
32) Benzene-d6	5.742	84	220162	3.909	ug/L	0.00
Spiked Amount 5.000	Range 70	- 125	Recovery	=	78.200%	
36) 1,2-Dichloropropane-d6	6.722	67	72412	4.128	ug/L	0.03
Spiked Amount 5.000	Range 60	- 140	Recovery	=	82.600%	
41) Toluene-d8	7.915	98	206767	3.888	ug/L	0.02
Spiked Amount 5.000	Range 70	- 130	Recovery	=	77.800%	
43) trans-1,3-Dichloroprop...	8.195	79	31236	4.052	ug/L	0.01
Spiked Amount 5.000	Range 55	- 130	Recovery	=	81.000%	
46) 2-Hexanone-d5	8.655	63	167568	38.193	ug/L	0.02
Spiked Amount 50.000	Range 45	- 130	Recovery	=	76.380%	
56) 1,1,2,2-Tetrachloroeth...	10.761	84	69701	3.900	ug/L	0.00
Spiked Amount 5.000	Range 65	- 120	Recovery	=	78.000%	
66) 1,2-Dichlorobenzene-d4	12.195	152	91307	4.085	ug/L	0.00
Spiked Amount 5.000	Range 80	- 120	Recovery	=	81.800%	
Target Compounds						
					Qvalue	
13) Acetone	2.777	43	27785m	14.445	ug/L	
19) 1,1-Dichloroethane	3.880	63	8297	0.458	ug/L	95
21) 2-Butanone	4.825	43	8915	2.438	ug/L	91
22) cis-1,2-Dichloroethene	4.678	96	2933	0.247	ug/L	96
33) Benzene	5.790	78	26155	0.580	ug/L	100
34) Trichloroethene	6.568	95	3221	0.272	ug/L	93
42) Toluene	7.983	91	61116	1.249	ug/L	98
47) Tetrachloroethene	8.562	164	13003	1.287	ug/L	97
52) Ethylbenzene	9.574	91	6731	0.129	ug/L	99
53) m,p-Xylene	9.697	106	4810	0.231	ug/L	96
54) o-Xylene	10.105	106	2771	0.138	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030422\
Data File : VU047334.D
Acq On : 04 Mar 2022 17:07
Operator : SY/MD
Sample : N1773-07
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFY14

Manual IntegrationsAPPROVED

Quant Time: Mar 04 23:23:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 04 23:20:39 2022
Response via : Initial Calibration

Reviewed By :John Carlone 03/07/2022
Supervised By :Mahesh Dadoda 03/07/2022

