

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030422\
 Data File : VU047337.D
 Acq On : 04 Mar 2022 18:18
 Operator : SY/MD
 Sample : N1810-01
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBD87

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047337.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	92	rBV	83697	95518	4.33%	1.153%
2	1.919	170	180	200	rBV	71455	98572	4.47%	1.190%
3	2.572	371	383	402	rVB	141018	231116	10.48%	2.790%
4	4.649	1011	1029	1066	rBV2	93665	370883	16.82%	4.477%
5	5.067	1143	1159	1183	rVB	125180	272756	12.37%	3.293%
6	5.729	1342	1365	1389	rBV2	255848	662541	30.04%	7.998%
7	6.250	1511	1527	1558	rBV	218845	413717	18.76%	4.994%
8	6.546	1603	1619	1651	rBV	1176584	2205298	100.00%	26.621%
9	6.694	1651	1665	1688	rVB	159278	313946	14.24%	3.790%
10	7.568	1923	1937	1956	rBV	87765	153140	6.94%	1.849%
11	7.899	2026	2040	2059	rBV	324993	557395	25.28%	6.729%
12	8.179	2114	2127	2141	rBV	55926	96436	4.37%	1.164%
13	8.555	2231	2244	2256	rVB	28001	47827	2.17%	0.577%
14	8.636	2256	2269	2308	rBV	451281	867356	39.33%	10.470%
15	9.417	2497	2512	2535	rBV	306510	517534	23.47%	6.247%
16	10.758	2918	2929	2945	rVB	151136	240582	10.91%	2.904%
17	11.812	3244	3257	3281	rVB	348705	551316	25.00%	6.655%
18	12.192	3362	3375	3394	rBV	346043	558167	25.31%	6.738%
19	16.886	4828	4835	4845	rBV2	21152	29917	1.36%	0.361%




Sum of corrected areas: 8284017

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030422\
Data File : VU047337.D
Acq On : 04 Mar 2022 18:18
Operator : SY/MD
Sample : N1810-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBD87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

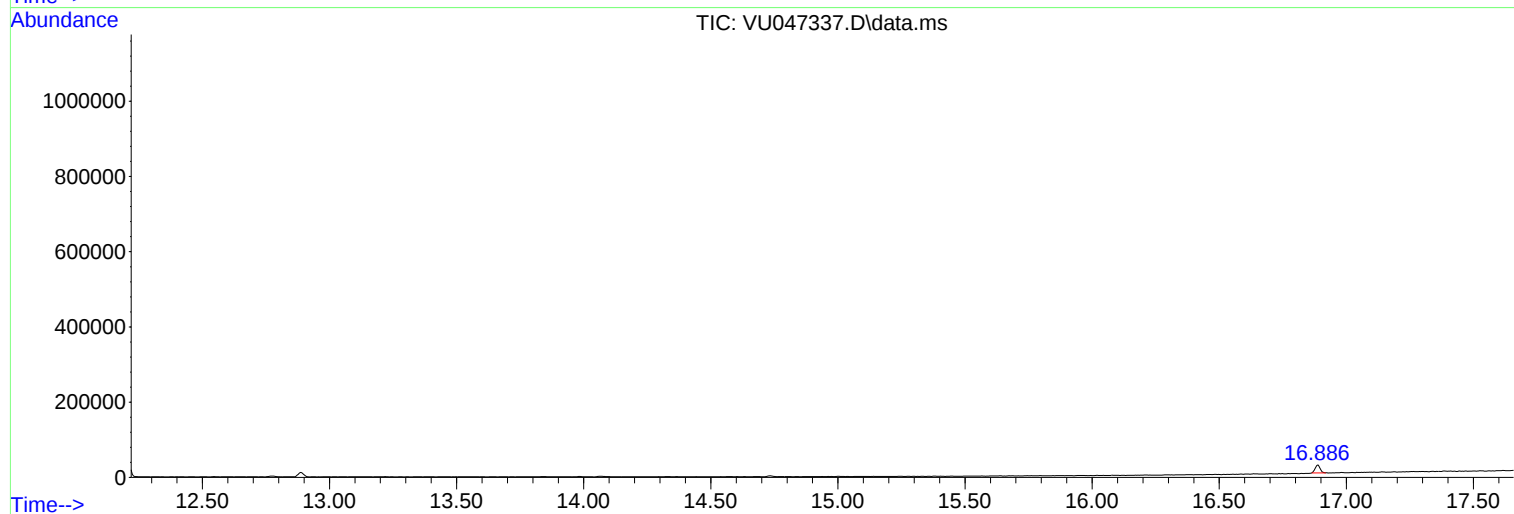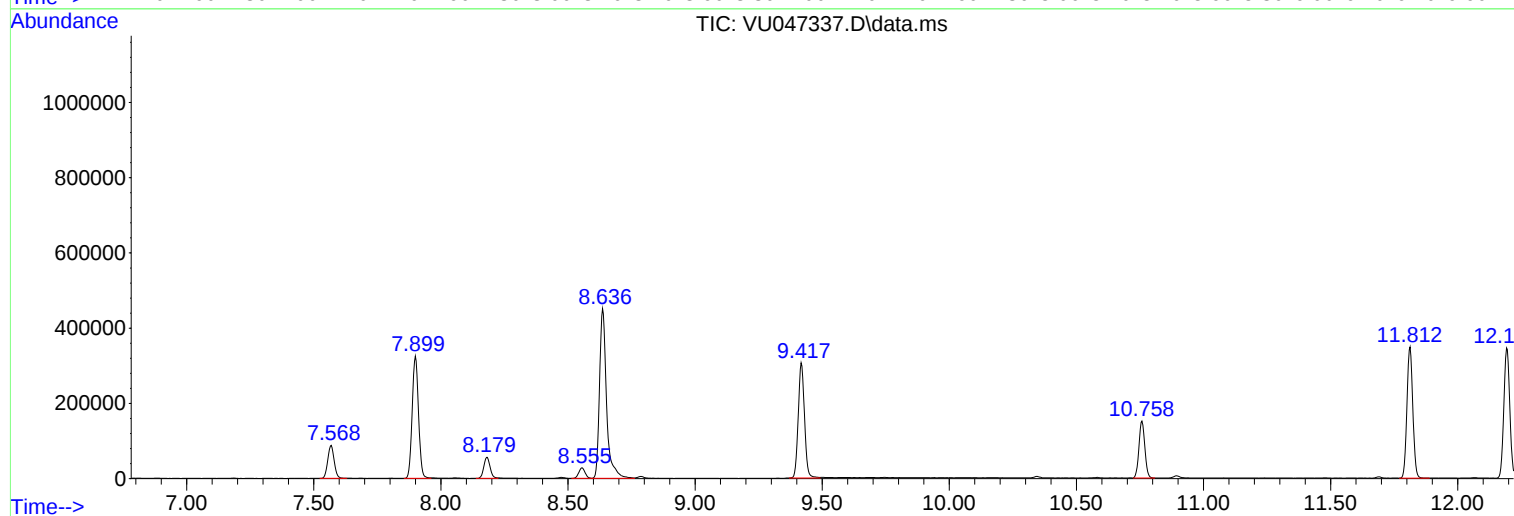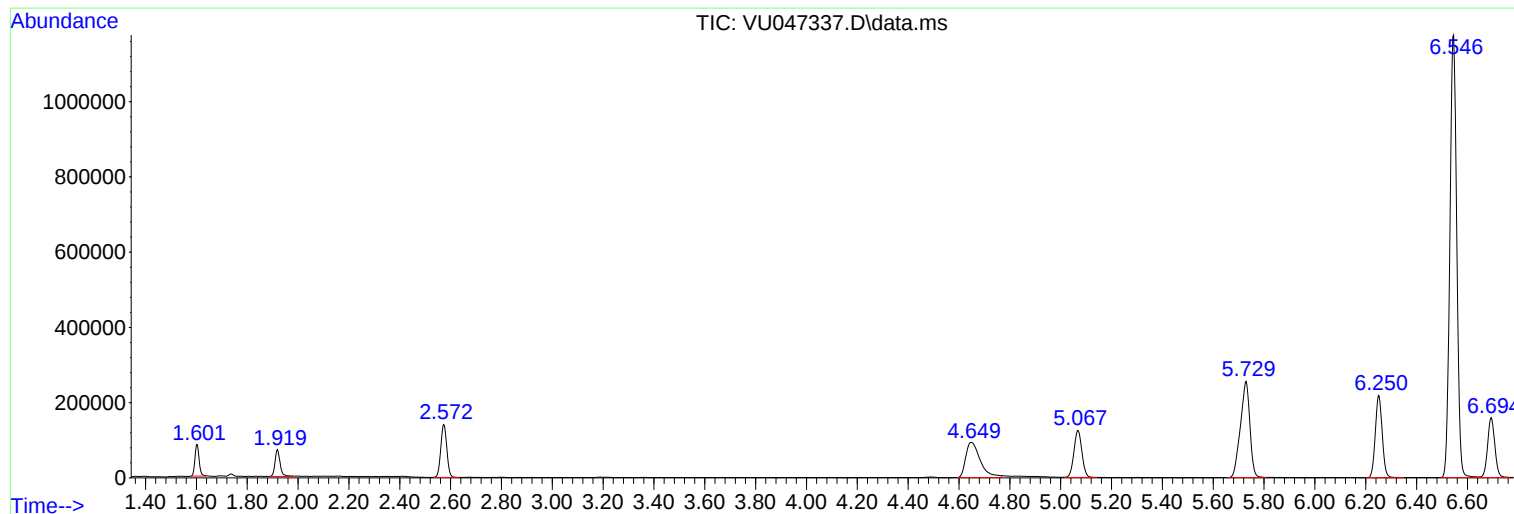

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030422\
Data File : VU047337.D
Acq On : 04 Mar 2022 18:18
Operator : SY/MD
Sample : N1810-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBD87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030422\
Data File : VU047337.D
Acq On : 04 Mar 2022 18:18
Operator : SY/MD
Sample : N1810-01
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBD87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
