

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
 Data File : VU047375.D
 Acq On : 07 Mar 2022 18:17
 Operator : SY/MD
 Sample : N1810-08
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBD94

Quant Time: Mar 08 03:03:23 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Fri Mar 04 23:20:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	6.253	114	180061	5.000	ug/L	0.00
28) Chlorobenzene-d5	9.420	117	170215	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.812	152	88820	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.601	65	52803	4.132	ug/L	0.00
Spiked Amount	5.000	Range	40 - 130	Recovery	=	82.600%
7) Chloroethane-d5	1.919	69	51805	4.859	ug/L	0.00
Spiked Amount	5.000	Range	65 - 130	Recovery	=	97.200%
11) 1,1-Dichloroethene-d2	2.572	65	22924	4.247	ug/L	0.00
Spiked Amount	5.000	Range	60 - 125	Recovery	=	85.000%
20) 2-Butanone-d5	4.639	46	196671	46.876	ug/L	0.00
Spiked Amount	50.000	Range	40 - 130	Recovery	=	93.760%
24) Chloroform-d	5.067	84	121410	5.142	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	102.800%
26) 1,2-Dichloroethane-d4	5.707	65	68932	5.202	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	104.000%
32) Benzene-d6	5.732	84	237937	4.963	ug/L	0.00
Spiked Amount	5.000	Range	70 - 125	Recovery	=	99.200%
36) 1,2-Dichloropropane-d6	6.694	67	80032	5.360	ug/L	0.00
Spiked Amount	5.000	Range	60 - 140	Recovery	=	107.200%
41) Toluene-d8	7.899	98	214826	4.746	ug/L	0.00
Spiked Amount	5.000	Range	70 - 130	Recovery	=	95.000%
43) trans-1,3-Dichloroprop...	8.179	79	31177	4.752	ug/L	0.00
Spiked Amount	5.000	Range	55 - 130	Recovery	=	95.000%
46) 2-Hexanone-d5	8.636	63	189452	50.735	ug/L	0.00
Spiked Amount	50.000	Range	45 - 130	Recovery	=	101.460%
56) 1,1,2,2-Tetrachloroeth...	10.758	84	74622	4.906	ug/L	0.00
Spiked Amount	5.000	Range	65 - 120	Recovery	=	98.200%
66) 1,2-Dichlorobenzene-d4	12.195	152	98744	5.673	ug/L	0.00
Spiked Amount	5.000	Range	80 - 120	Recovery	=	113.400%
Target Compounds						Qvalue
34) Trichloroethene	6.546	95	44823	4.439	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
Data File : VU047375.D
Acq On : 07 Mar 2022 18:17
Operator : SY/MD
Sample : N1810-08
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBD94


Quant Time: Mar 08 03:03:23 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Fri Mar 04 23:20:39 2022
Response via : Initial Calibration

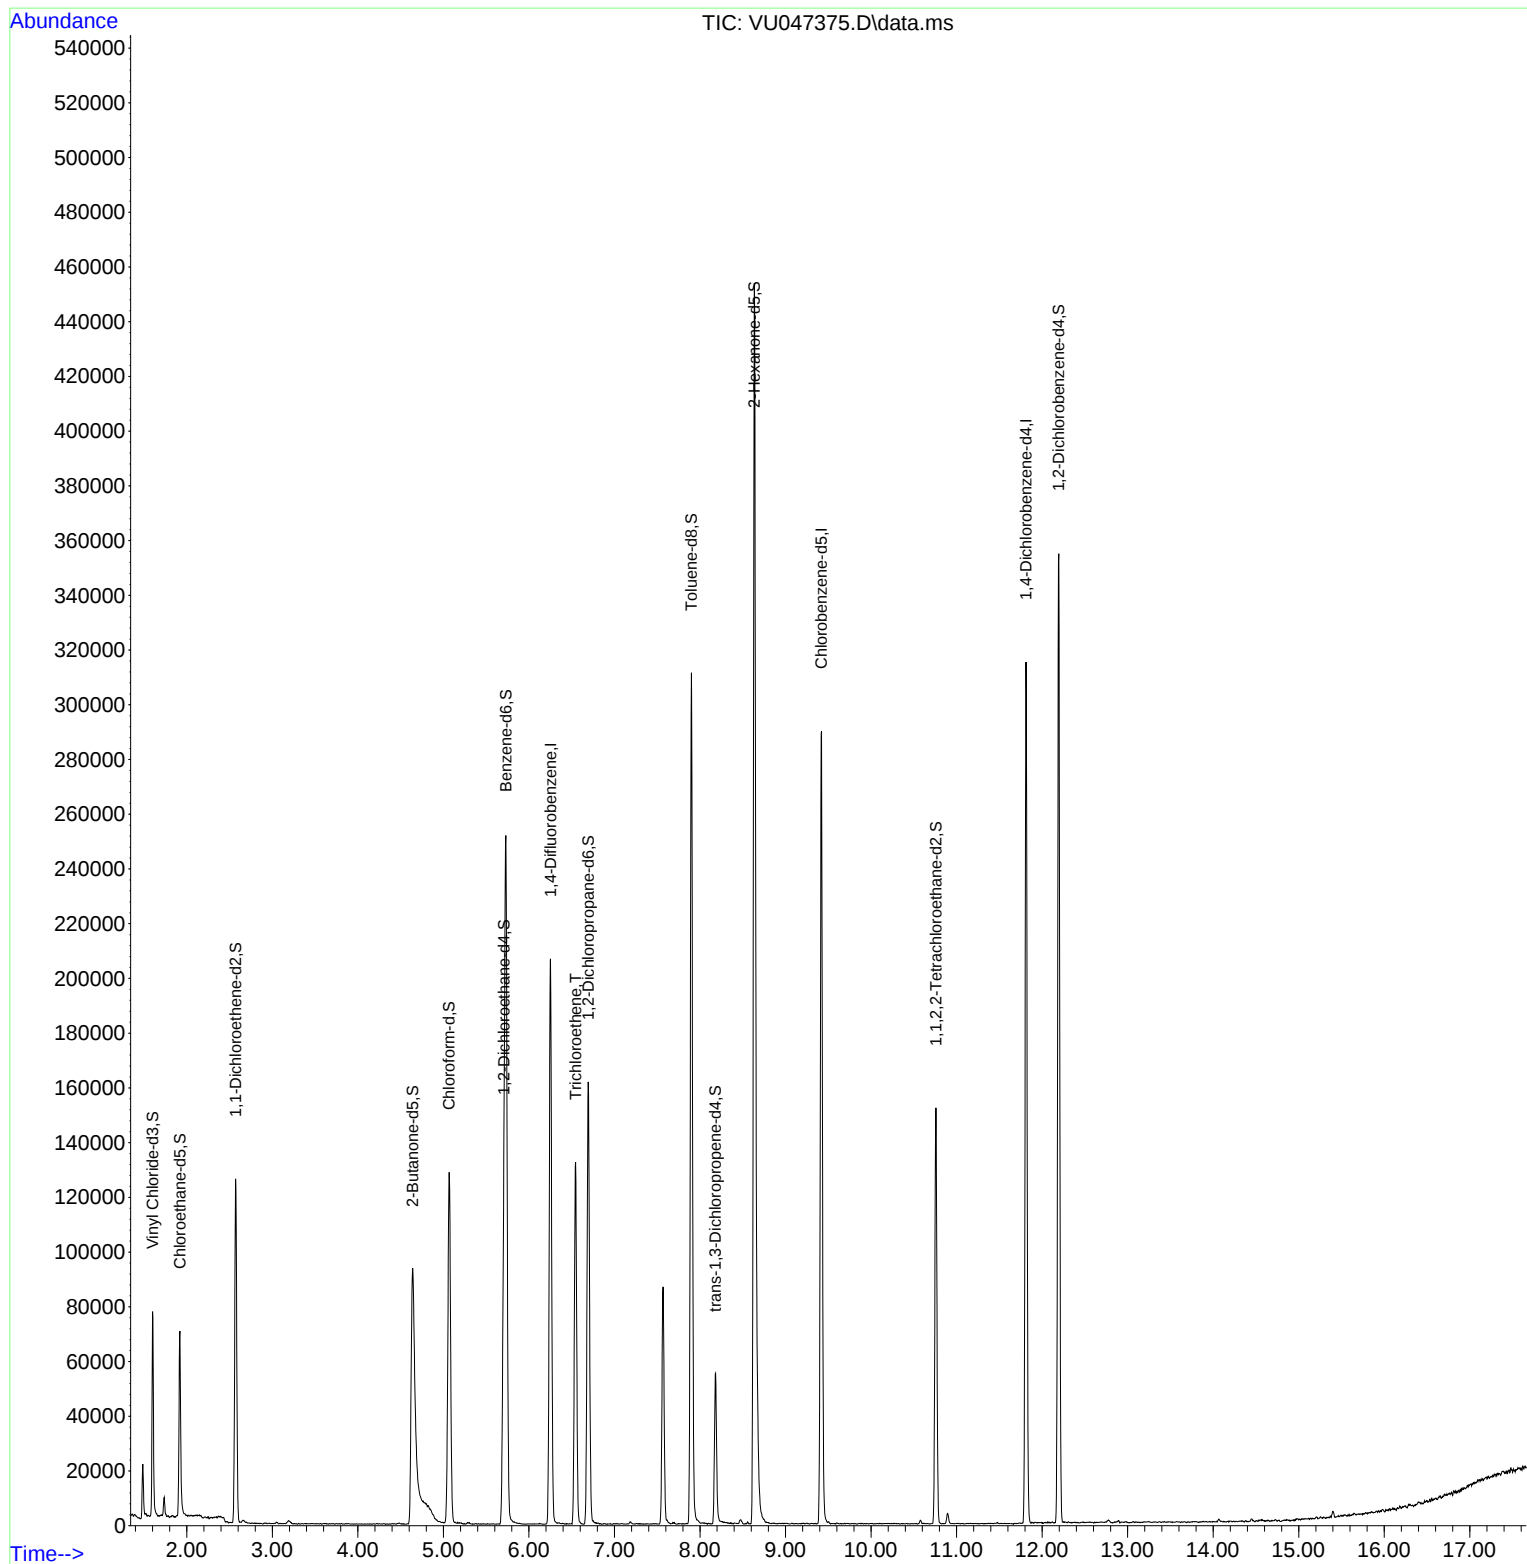

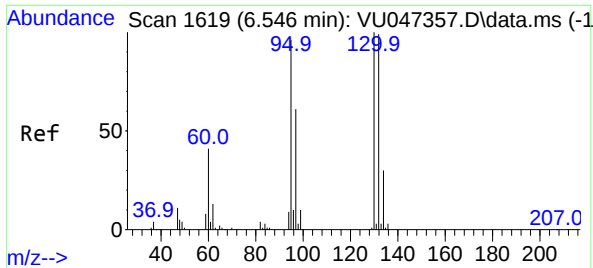

#34
 Trichloroethene
 Concen: 4.439 ug/L
 RT: 6.546 min Scan# 1
 Delta R.T. 0.000 min
 Lab File: VU047375.D
 Acq: 07 Mar 2022 18:17

Instrument :
 MSVOA_U
 ClientSampleId :
 GBD94

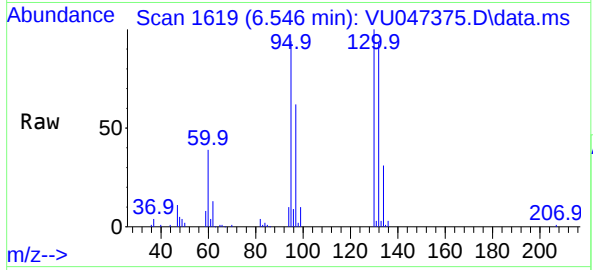

Tgt Ion: 95 Resp: 44823

Ion	Ratio	Lower	Upper
95	100		
97	65.7	46.5	86.5
132	99.9	65.1	120.9
130	106.8	67.3	124.9

