

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
 Data File : VU047364.D
 Acq On : 07 Mar 2022 13:57
 Operator : SY/MD
 Sample : N1822-02
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AA4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047364.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	74	81	96	rBV	83555	99434	5.13%	1.135%
2	1.919	171	180	200	rBV	76232	102529	5.29%	1.170%
3	2.572	371	383	397	rBV	146890	238096	12.29%	2.717%
4	4.642	1010	1027	1066	rBV2	106301	389166	20.08%	4.441%
5	5.070	1143	1160	1185	rVB2	148808	354657	18.30%	4.047%
6	5.729	1344	1365	1391	rBV2	284846	744430	38.42%	8.495%
7	6.250	1513	1527	1549	rBV	235588	449183	23.18%	5.126%
8	6.694	1651	1665	1686	rBV	181610	351587	18.15%	4.012%
9	7.568	1924	1937	1965	rBV	99751	175819	9.07%	2.006%
10	7.899	2021	2040	2066	rBV	357076	620961	32.05%	7.086%
11	8.182	2113	2128	2148	rBV	63035	109883	5.67%	1.254%
12	8.555	2229	2244	2258	rBV	1151976	1937601	100.00%	22.112%
13	8.636	2258	2269	2310	rVB	500990	988718	51.03%	11.283%
14	9.417	2500	2512	2534	rBV	330826	552080	28.49%	6.300%
15	10.758	2917	2929	2948	rVB	169045	274827	14.18%	3.136%
16	11.812	3244	3257	3274	rBV	378236	603883	31.17%	6.892%
17	12.195	3363	3376	3394	rBV	395228	637751	32.91%	7.278%
18	15.401	4363	4373	4382	rBV	39410	56564	2.92%	0.646%
19	15.976	4545	4552	4565	rVB2	23804	32371	1.67%	0.369%
20	16.294	4643	4651	4662	rVB	31015	43171	2.23%	0.493%




Sum of corrected areas: 8762711

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
Data File : VU047364.D
Acq On : 07 Mar 2022 13:57
Operator : SY/MD
Sample : N1822-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

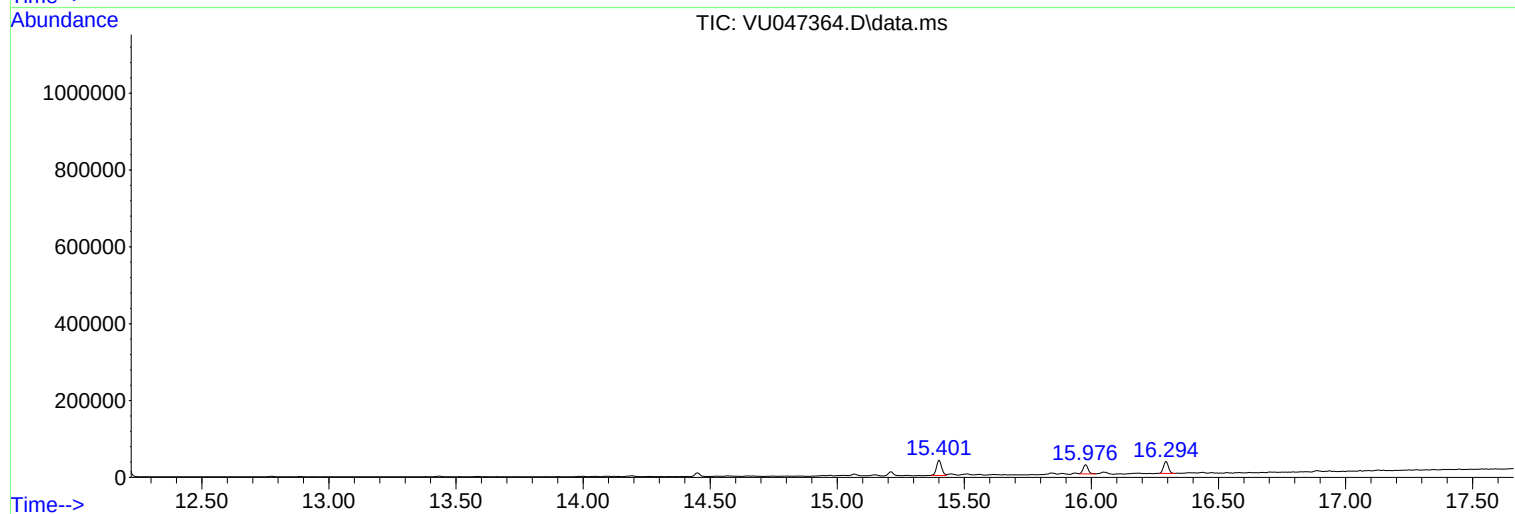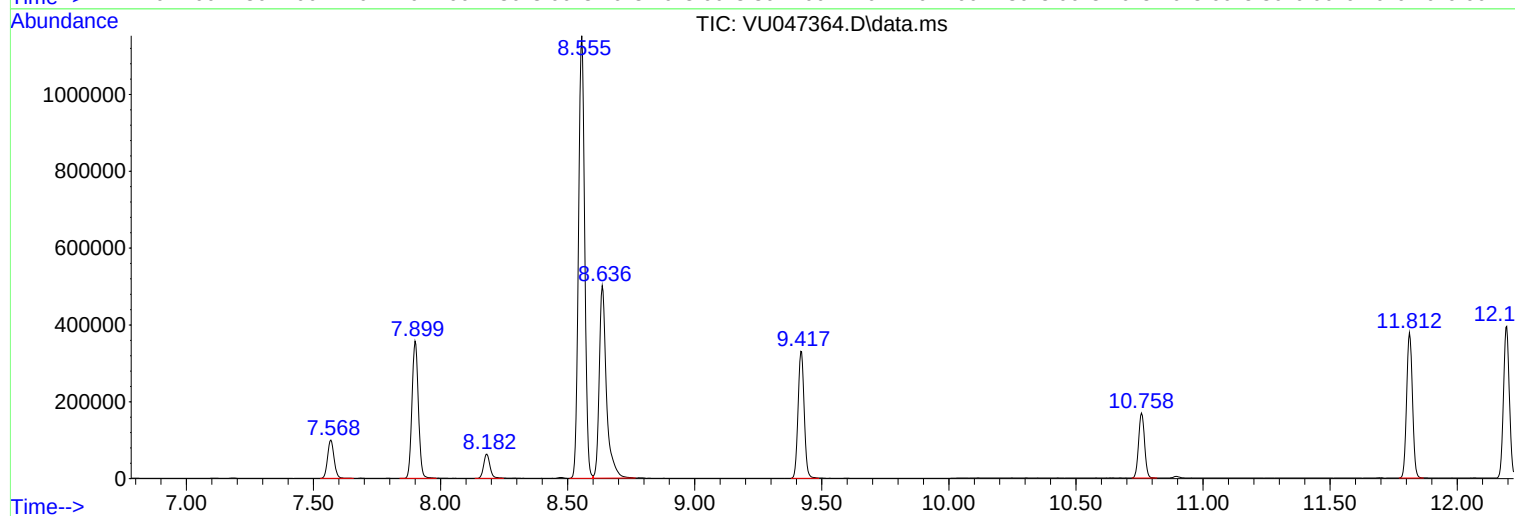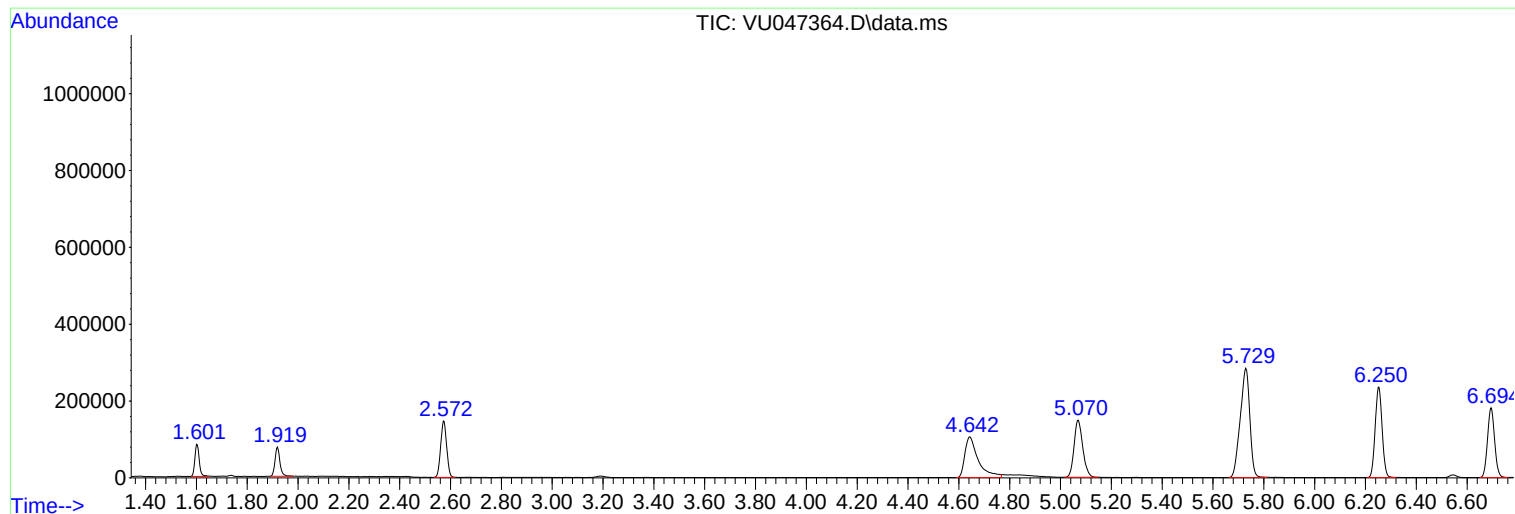

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
Data File : VU047364.D
Acq On : 07 Mar 2022 13:57
Operator : SY/MD
Sample : N1822-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
Data File : VU047364.D
Acq On : 07 Mar 2022 13:57
Operator : SY/MD
Sample : N1822-02
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
