

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
 Data File : VU047365.D
 Acq On : 07 Mar 2022 14:21
 Operator : SY/MD
 Sample : N1822-03
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 C0AA8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VU047365.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.382	3	13	22	rVB2	6627	11018	1.15%	0.167%
2	1.527	50	58	73	rBV	137291	176074	18.41%	2.667%
3	1.604	74	82	96	rVV	86595	98191	10.26%	1.487%
4	1.919	172	180	196	rVB	75659	98603	10.31%	1.494%
5	2.572	371	383	400	rVB	147867	238173	24.90%	3.608%
6	3.369	619	631	646	rVB2	8425	19027	1.99%	0.288%
7	4.642	1009	1027	1058	rBV	94783	327866	34.27%	4.967%
8	5.067	1143	1159	1182	rBV	144719	314573	32.88%	4.765%
9	5.729	1344	1365	1387	rBV2	280483	737309	77.08%	11.169%
10	6.253	1513	1528	1546	rBV	235284	446502	46.68%	6.764%
11	6.694	1649	1665	1688	rBV	182117	353779	36.98%	5.359%
12	7.568	1922	1937	1954	rBV	100589	173730	18.16%	2.632%
13	7.899	2026	2040	2059	rBV	349158	604336	63.18%	9.154%
14	8.182	2115	2128	2140	rBV	63638	108147	11.31%	1.638%
15	8.555	2236	2244	2255	rVB4	6688	10731	1.12%	0.163%
16	8.636	2255	2269	2301	rBV	482021	956599	100.00%	14.491%
17	9.420	2500	2513	2534	rBV	319544	534799	55.91%	8.101%
18	10.758	2917	2929	2947	rVB	166109	270185	28.24%	4.093%
19	11.812	3244	3257	3272	rBV	326082	515127	53.85%	7.803%
20	12.195	3363	3376	3396	rVB	342902	548597	57.35%	8.310%
21	15.401	4365	4373	4381	rBV	22021	28967	3.03%	0.439%
22	15.976	4546	4552	4559	rBV2	9985	12076	1.26%	0.183%
23	16.291	4644	4650	4659	rBV	13731	17115	1.79%	0.259%




Sum of corrected areas: 6601524

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
Data File : VU047365.D
Acq On : 07 Mar 2022 14:21
Operator : SY/MD
Sample : N1822-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

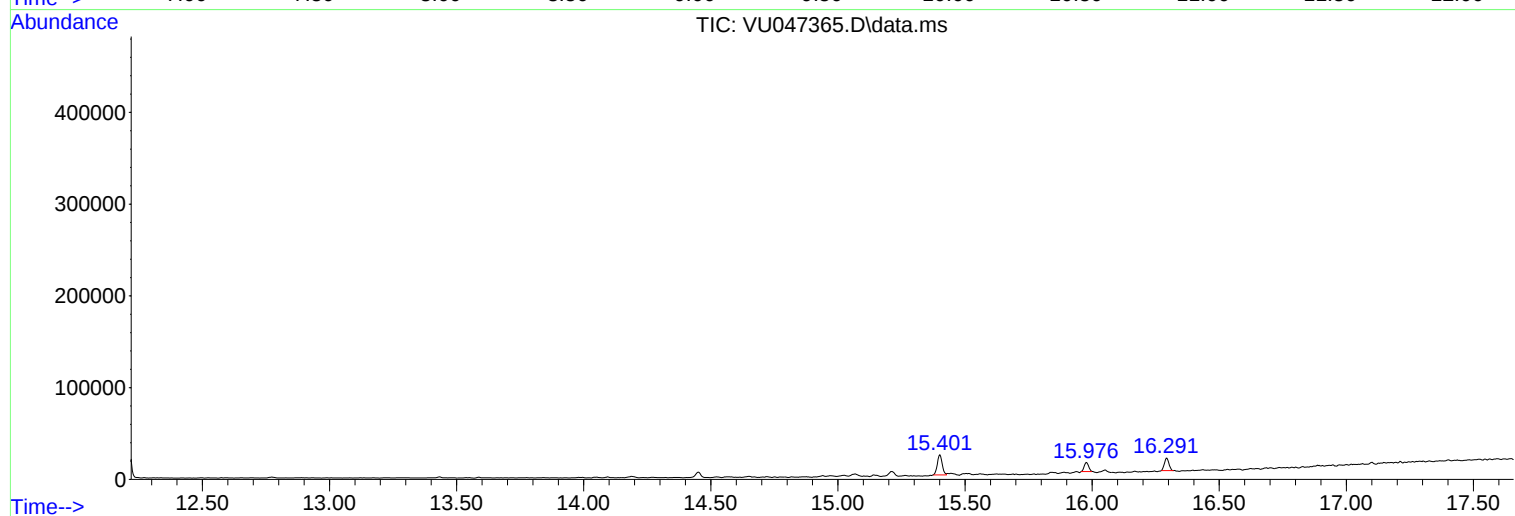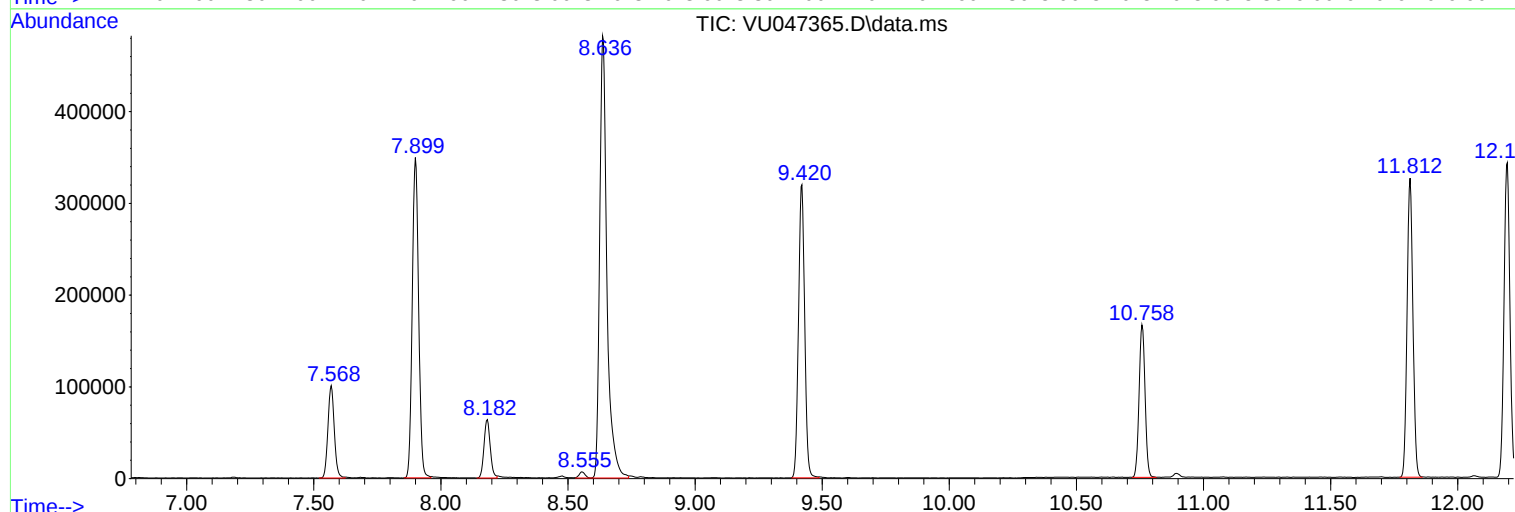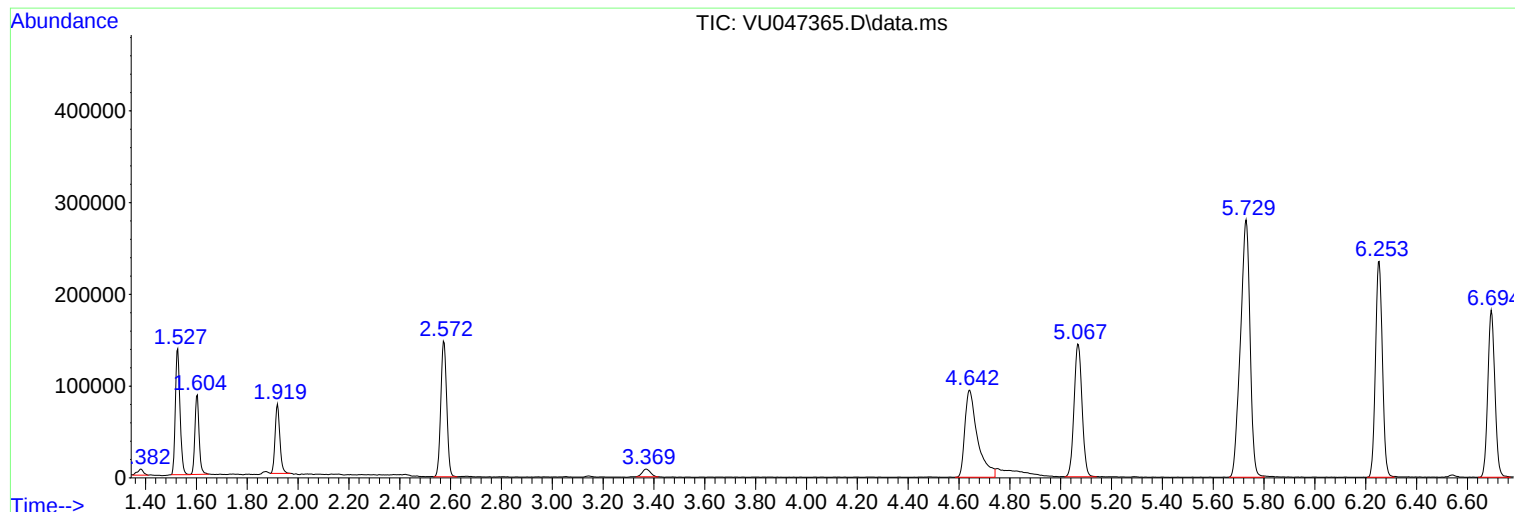

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
Data File : VU047365.D
Acq On : 07 Mar 2022 14:21
Operator : SY/MD
Sample : N1822-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
Data File : VU047365.D
Acq On : 07 Mar 2022 14:21
Operator : SY/MD
Sample : N1822-03
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
C0AA8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc