

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
 Data File : VU047368.D
 Acq On : 07 Mar 2022 15:32
 Operator : SY/MD
 Sample : N1773-09DL 40X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 BFY16DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047368.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	96	rBV	78257	94149	10.22%	1.235%
2	1.919	171	180	200	rBV	72336	99191	10.77%	1.301%
3	2.572	372	383	398	rBV	141404	230082	24.98%	3.019%
4	3.051	522	532	547	rBV2	5296	10279	1.12%	0.135%
5	4.642	1008	1027	1060	rBV3	96969	385076	41.80%	5.052%
6	5.070	1142	1160	1180	rBV	135742	300501	32.62%	3.943%
7	5.729	1344	1365	1387	rBV2	268550	702243	76.23%	9.213%
8	6.253	1504	1528	1549	rBV	212413	400792	43.51%	5.258%
9	6.546	1605	1619	1636	rBV	382623	721496	78.32%	9.466%
10	6.694	1651	1665	1682	rBV	170877	332055	36.05%	4.357%
11	7.568	1924	1937	1959	rVB	92891	163376	17.74%	2.143%
12	7.899	2025	2040	2062	rBV	334304	579751	62.94%	7.606%
13	8.182	2116	2128	2141	rBV	59565	102092	11.08%	1.339%
14	8.555	2231	2244	2257	rBV	404344	678013	73.60%	8.895%
15	8.636	2257	2269	2308	rVB	471869	921189	100.00%	12.086%
16	9.417	2500	2512	2532	rBV	298404	494626	53.69%	6.489%
17	10.758	2917	2929	2946	rVB	162569	259970	28.22%	3.411%
18	10.896	2960	2972	2984	rVB2	6842	11244	1.22%	0.148%
19	11.812	3245	3257	3273	rBV	329310	520885	56.54%	6.834%
20	12.195	3363	3376	3393	rBV	372399	603638	65.53%	7.920%
21	15.401	4364	4373	4382	rBV3	7215	11372	1.23%	0.149%




Sum of corrected areas: 7622020

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
Data File : VU047368.D
Acq On : 07 Mar 2022 15:32
Operator : SY/MD
Sample : N1773-09DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFY16DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

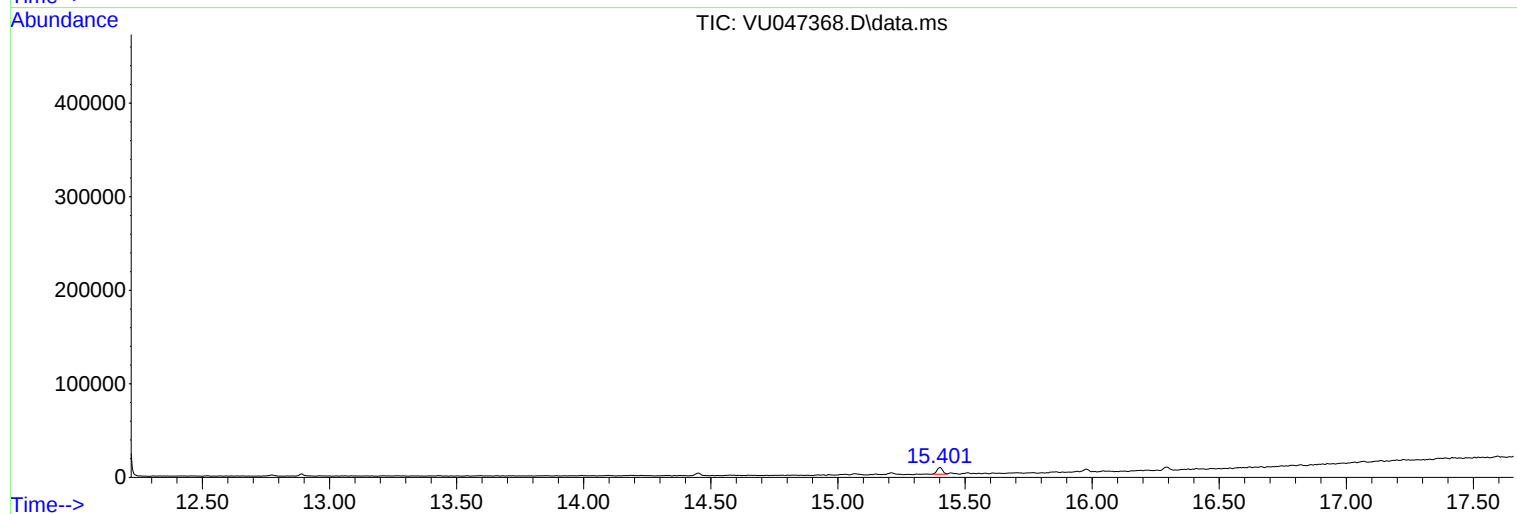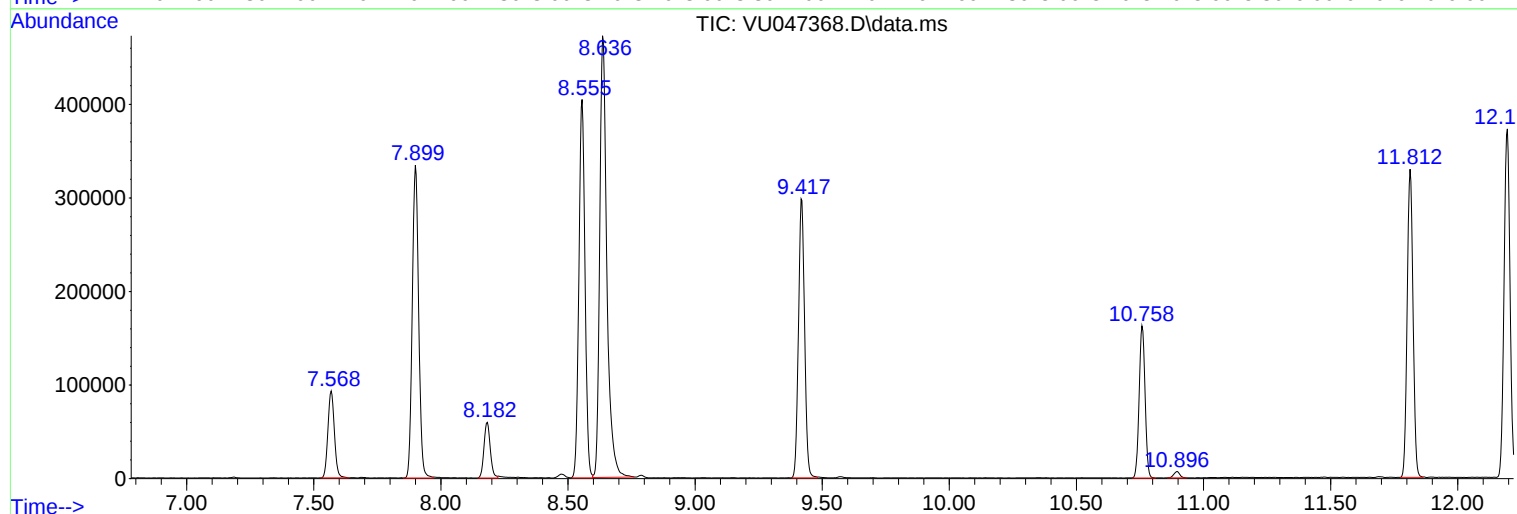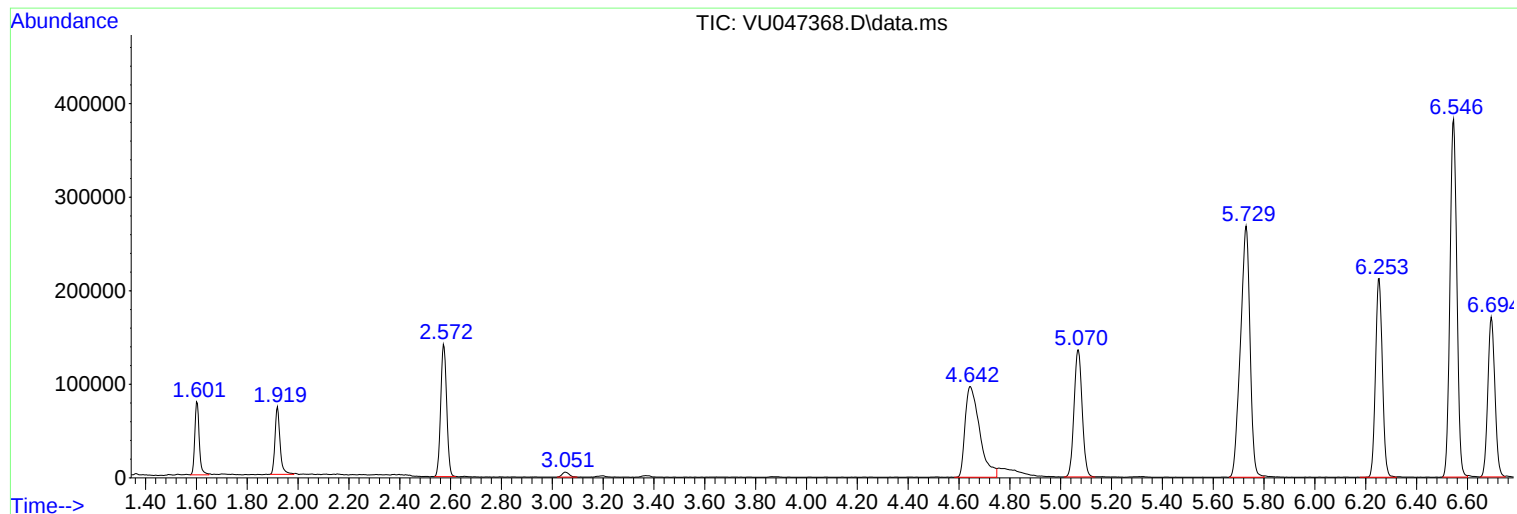

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
Data File : VU047368.D
Acq On : 07 Mar 2022 15:32
Operator : SY/MD
Sample : N1773-09DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFY16DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
Data File : VU047368.D
Acq On : 07 Mar 2022 15:32
Operator : SY/MD
Sample : N1773-09DL 40X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
BFY16DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc