

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
 Data File : VU047378.D
 Acq On : 07 Mar 2022 19:28
 Operator : SY/MD
 Sample : N1810-18DL 5X
 Misc : 25.0mL/MSVOA_U/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_U
 ClientSampleId :
 GBDA5DL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VU047378.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.601	73	81	108	rVB	58563	84225	9.30%	1.335%
2	1.916	171	179	207	rBV	56006	98616	10.89%	1.563%
3	2.565	369	381	395	rVB	128715	206413	22.79%	3.272%
4	3.051	520	532	549	rVB	5449	10234	1.13%	0.162%
5	3.189	562	575	594	rBV	5167	12650	1.40%	0.201%
6	4.649	1009	1029	1062	rBV	77621	318342	35.15%	5.046%
7	5.067	1143	1159	1180	rBV	125058	275715	30.44%	4.370%
8	5.726	1343	1364	1392	rBV2	252431	655956	72.42%	10.397%
9	6.250	1513	1527	1552	rBV	207414	393320	43.42%	6.234%
10	6.543	1605	1618	1633	rBV	205887	386148	42.63%	6.121%
11	6.694	1651	1665	1692	rVB	161159	313690	34.63%	4.972%
12	7.568	1924	1937	1954	rBV	83568	146815	16.21%	2.327%
13	7.899	2027	2040	2060	rBV	306049	534773	59.04%	8.476%
14	8.182	2108	2128	2149	rBV	52891	95464	10.54%	1.513%
15	8.649	2258	2273	2303	rBV	437815	905746	100.00%	14.357%
16	9.420	2500	2513	2532	rBV	297848	501403	55.36%	7.948%
17	10.761	2917	2930	2944	rVB	160341	254536	28.10%	4.035%
18	11.812	3245	3257	3274	rBV	341647	540815	59.71%	8.572%
19	12.195	3363	3376	3394	rBV	359449	574078	63.38%	9.099%




Sum of corrected areas: 6308939

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
Data File : VU047378.D
Acq On : 07 Mar 2022 19:28
Operator : SY/MD
Sample : N1810-18DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBDA5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

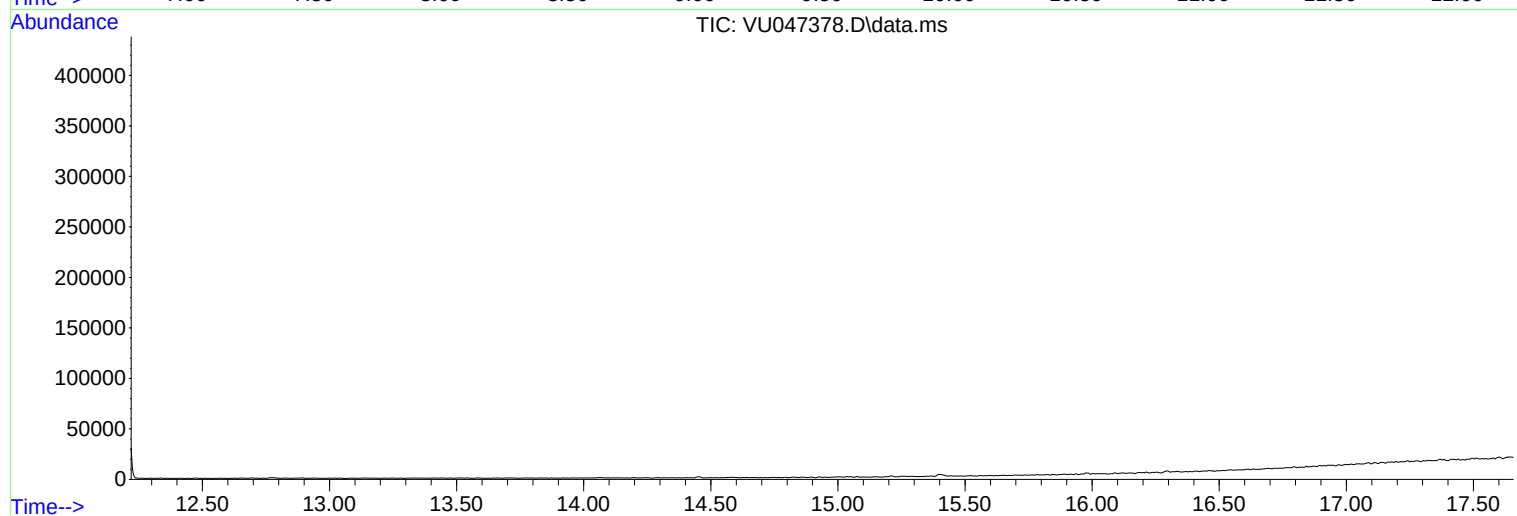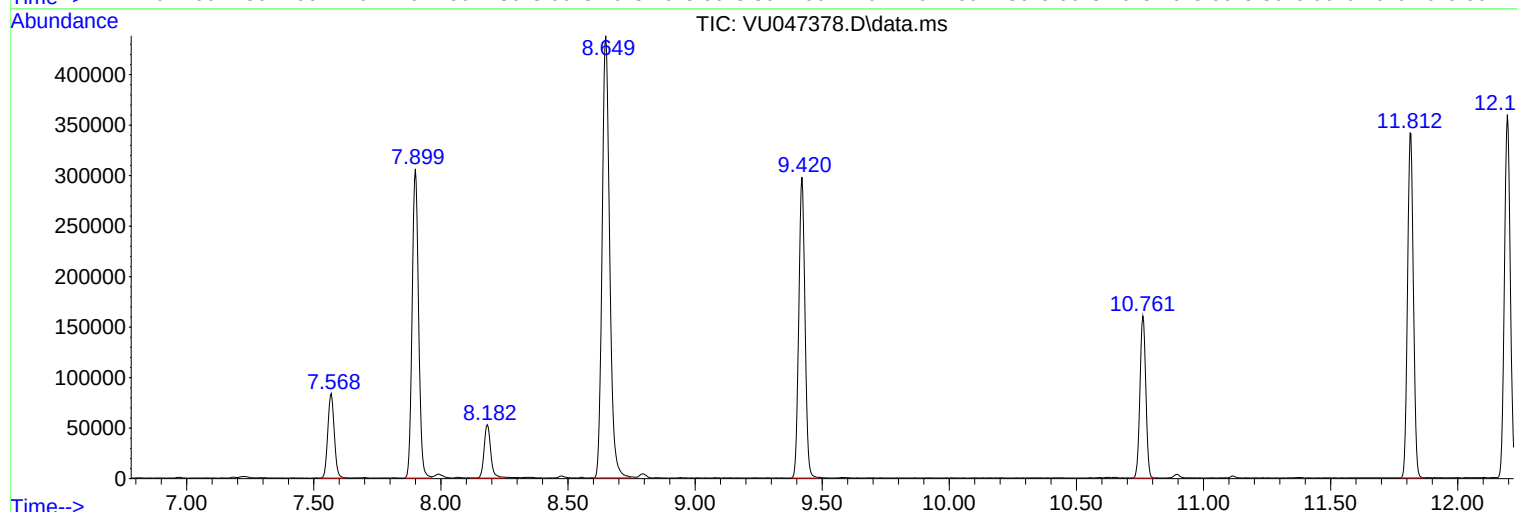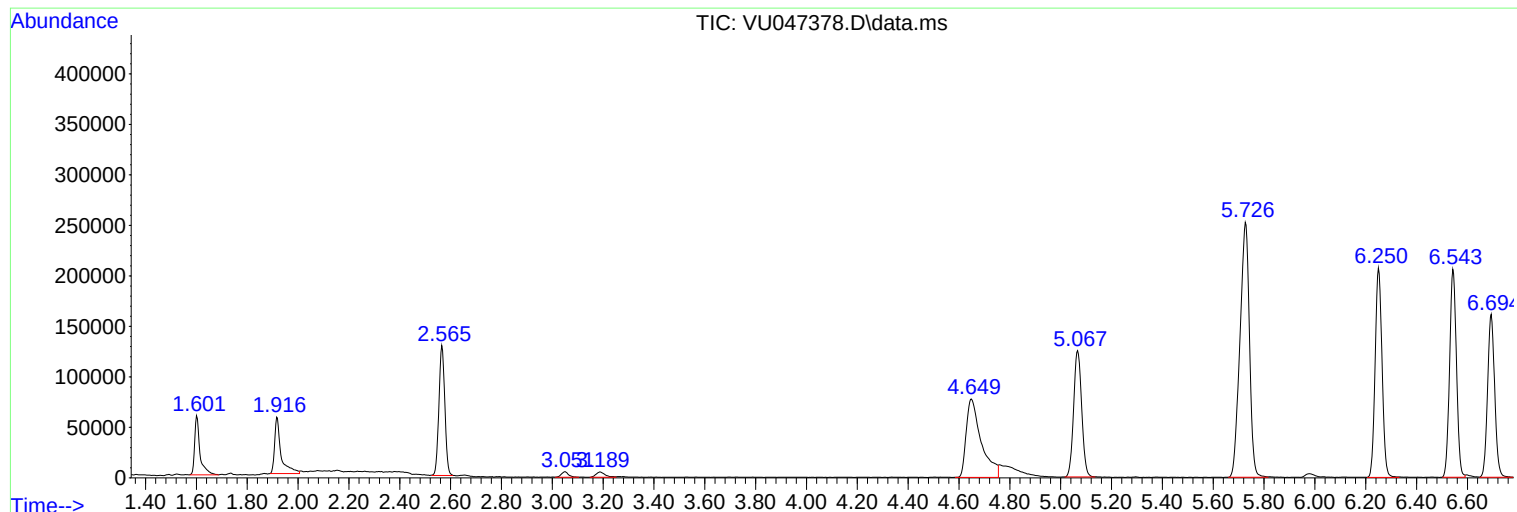

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
Data File : VU047378.D
Acq On : 07 Mar 2022 19:28
Operator : SY/MD
Sample : N1810-18DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBDA5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_U\Data\VU030722\
Data File : VU047378.D
Acq On : 07 Mar 2022 19:28
Operator : SY/MD
Sample : N1810-18DL 5X
Misc : 25.0mL/MSVOA_U/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_U
ClientSampleId :
GBDA5DL

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_U\Method\SFAMUTR030422WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc